

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106206

Date: 11/25/2013

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 13200

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:37
INTERNAL STANDARD	VERIFIED	08:37
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	08:38
BLANK TEST	0.00	08:38
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	08:39
BLANK TEST	0.00	08:39
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	08:40
BLANK TEST	0.00	08:40

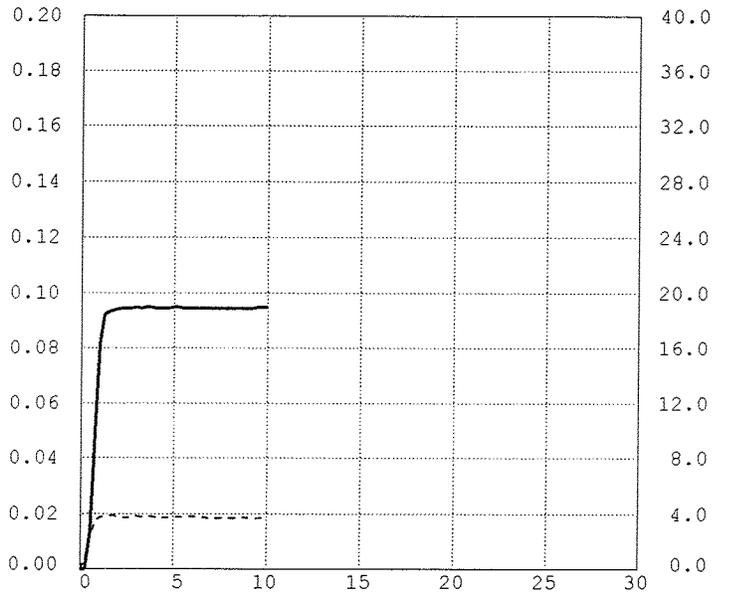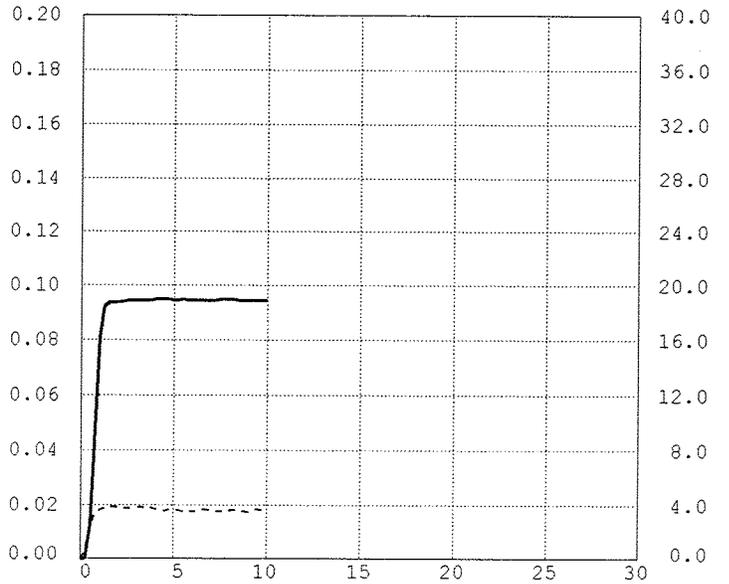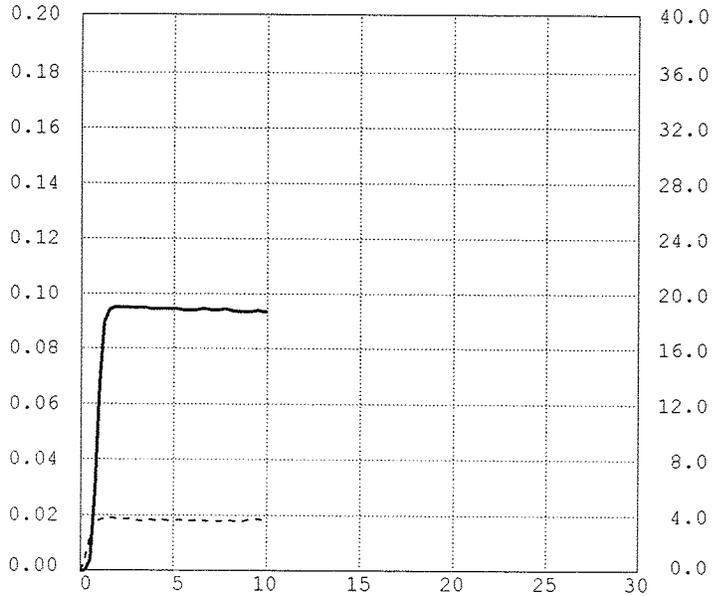

*Handwritten signature and notes:*  
P. Ch... #248 11/25/13 0841