

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106206

Date: 12/01/2013

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 13260

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:26
INTERNAL STANDARD	VERIFIED	12:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	12:26
BLANK TEST	0.00	12:27
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:27
BLANK TEST	0.00	12:28
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:28
BLANK TEST	0.00	12:29

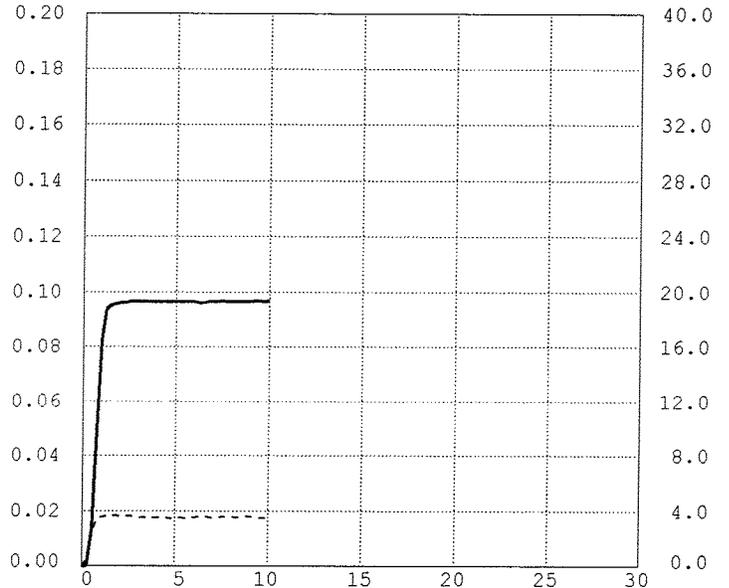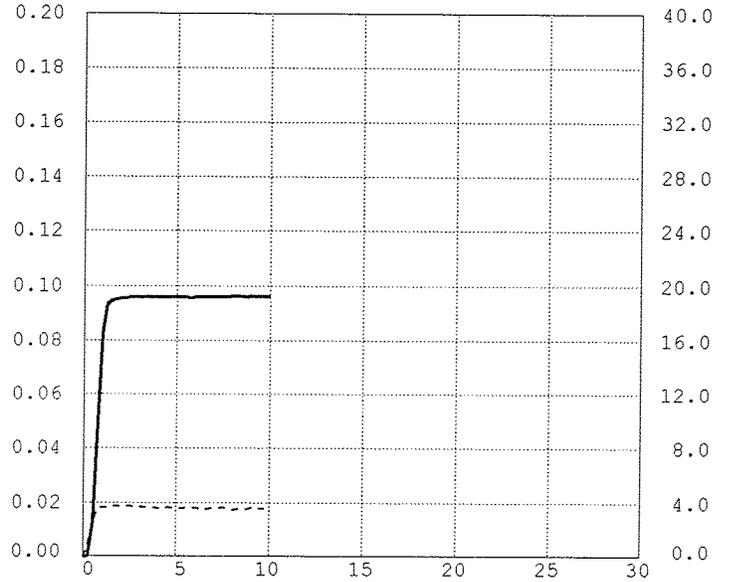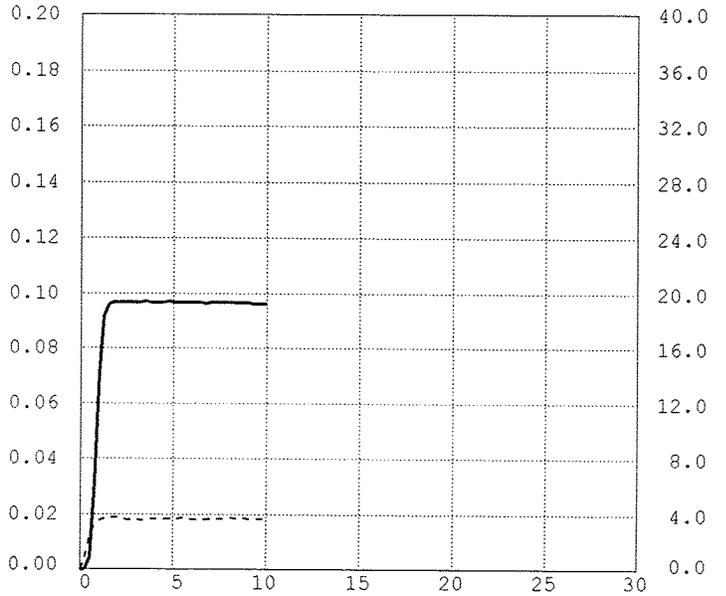

*Charles B. Geisler*  
#248 12/01/13