

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 12/16/2013

Operator Name: RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13260

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:21
INTERNAL STANDARD	VERIFIED	23:21
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	23:22
BLANK TEST	0.00	23:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:23
BLANK TEST	0.00	23:23
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	23:24
BLANK TEST	0.00	23:24

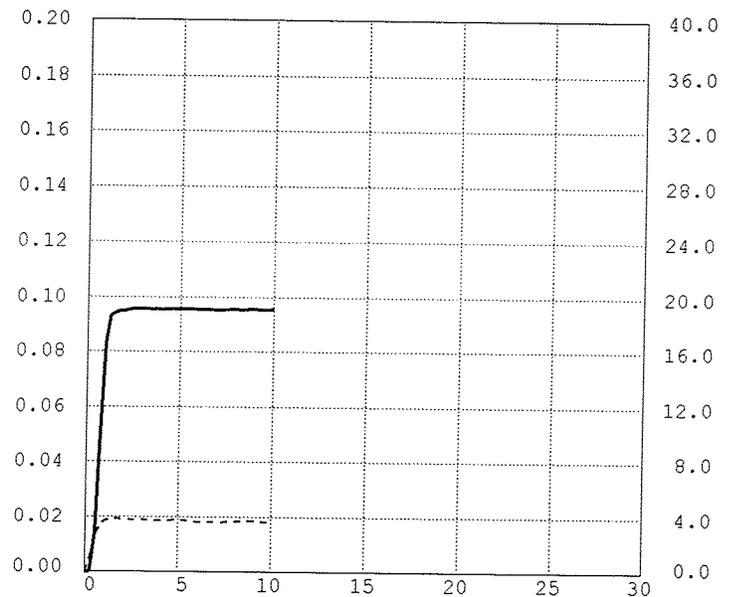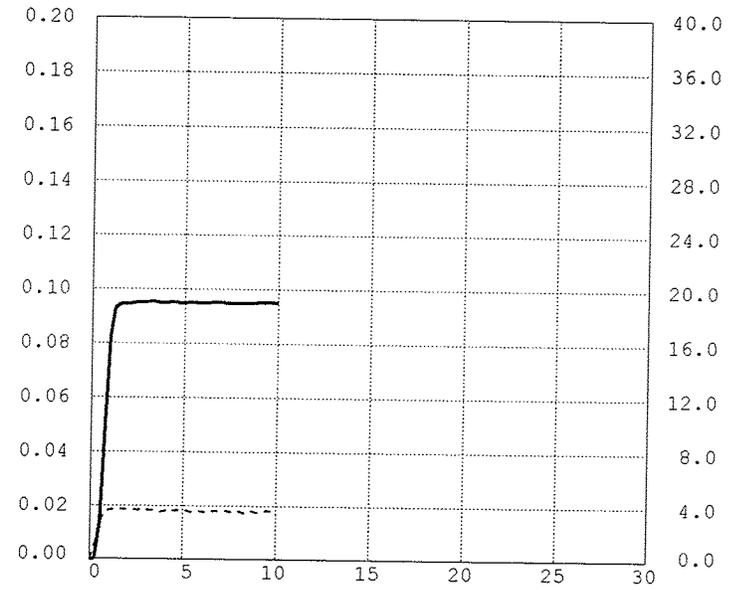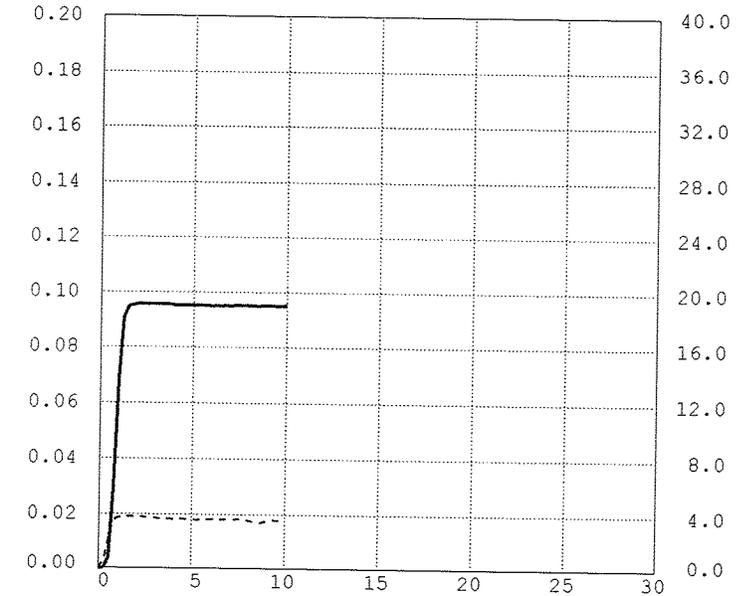

See Ref of ~~Printout~~ W050 #162 12-16-13