

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106206

Date: 02/25/2014

Operator Name: RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13320

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:47
INTERNAL STANDARD	VERIFIED	01:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:47
BLANK TEST	0.00	01:48
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:49
BLANK TEST	0.00	01:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:50
BLANK TEST	0.00	01:50

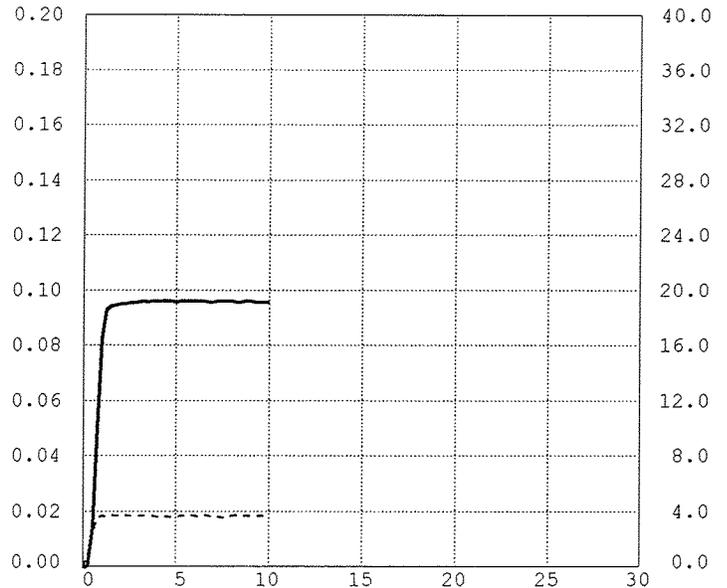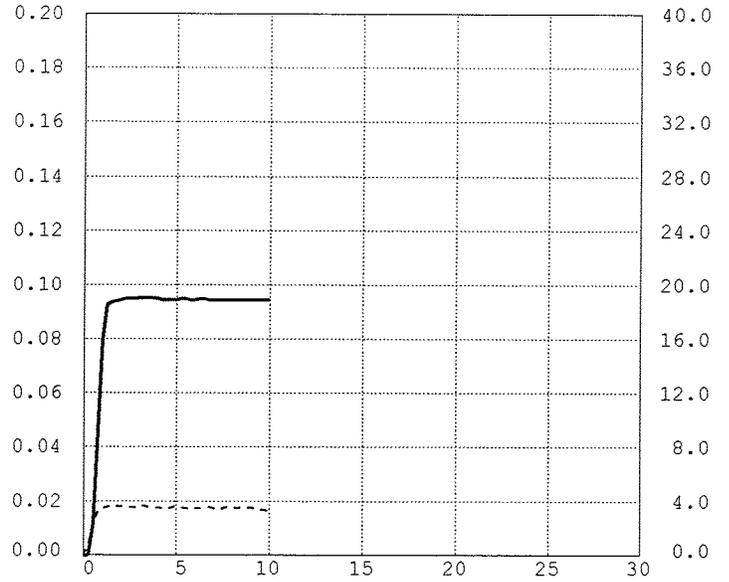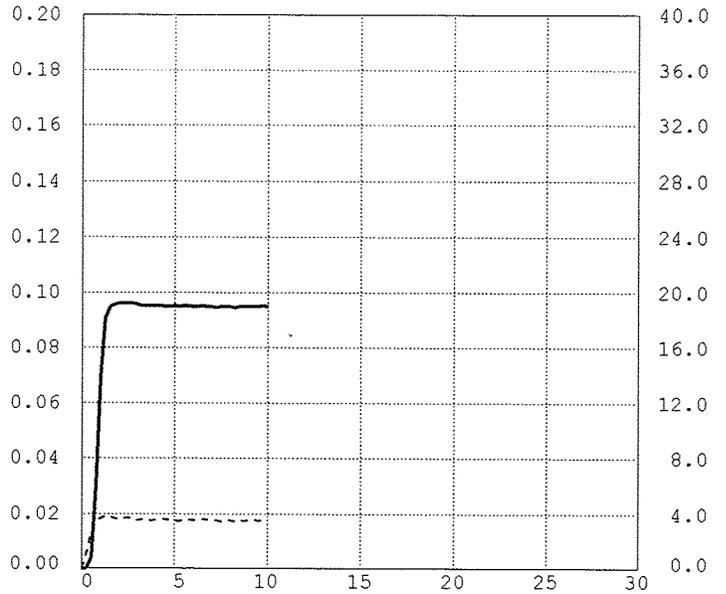

SGS Ray Bartlett W250 #162 02-25-14