

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/16/2009

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 09200

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:43
INTERNAL STANDARD	VERIFIED	09:44
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	09:44
BLANK TEST	0.00	09:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:45
BLANK TEST	0.00	09:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:46
BLANK TEST	0.00	09:47

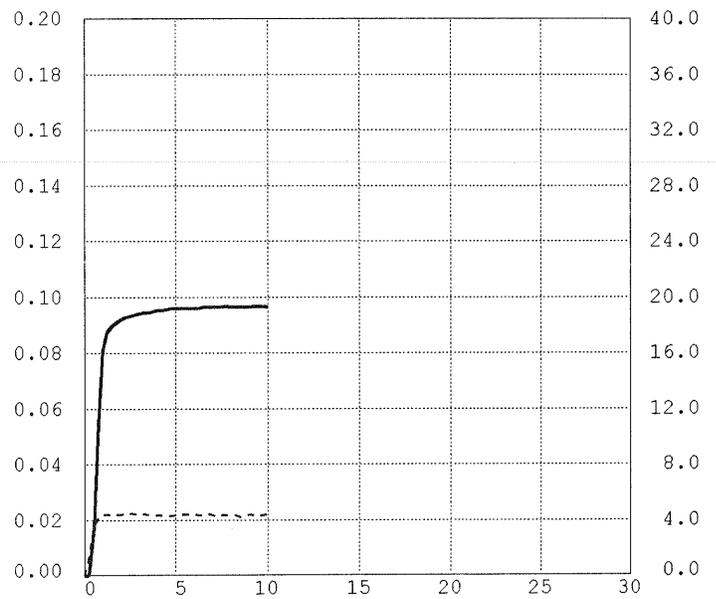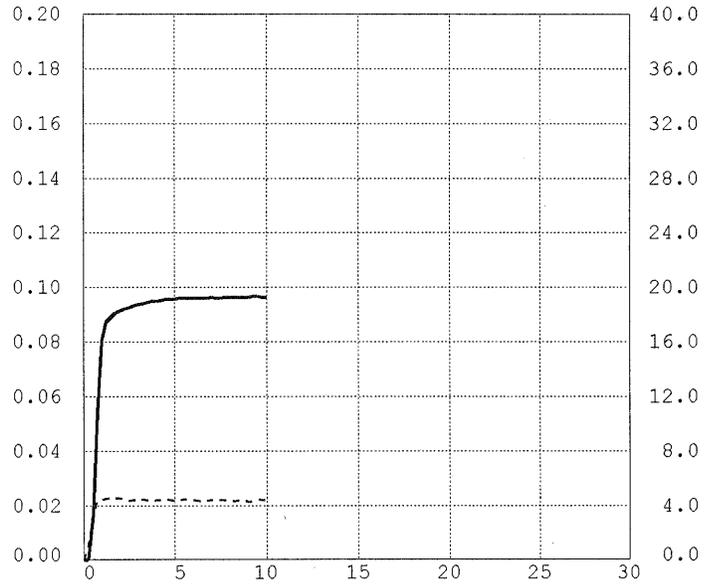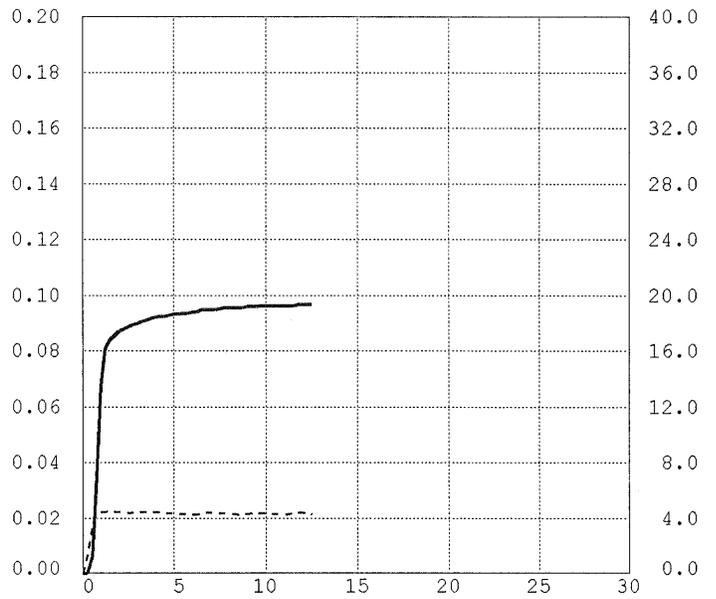

Charles B Geisler