

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 11/25/2009

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 09200

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:25
INTERNAL STANDARD	VERIFIED	18:25
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	18:26
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	18:27
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.09	18:28
BLANK TEST	0.00	18:28

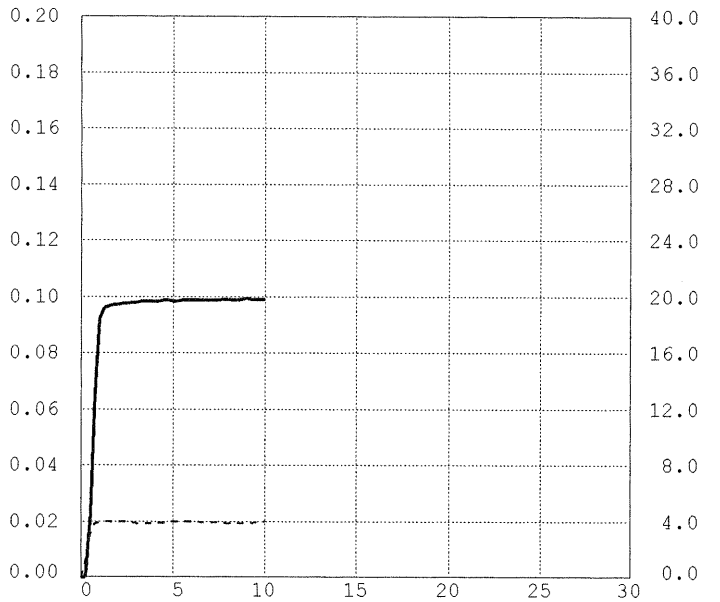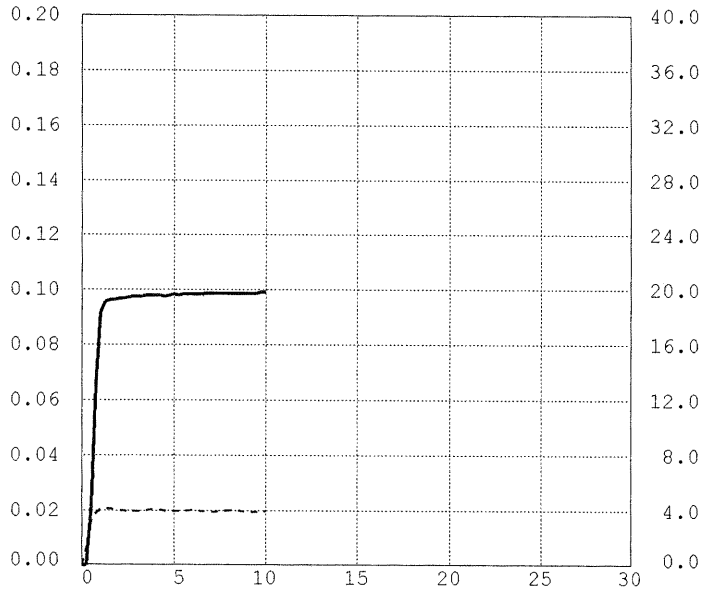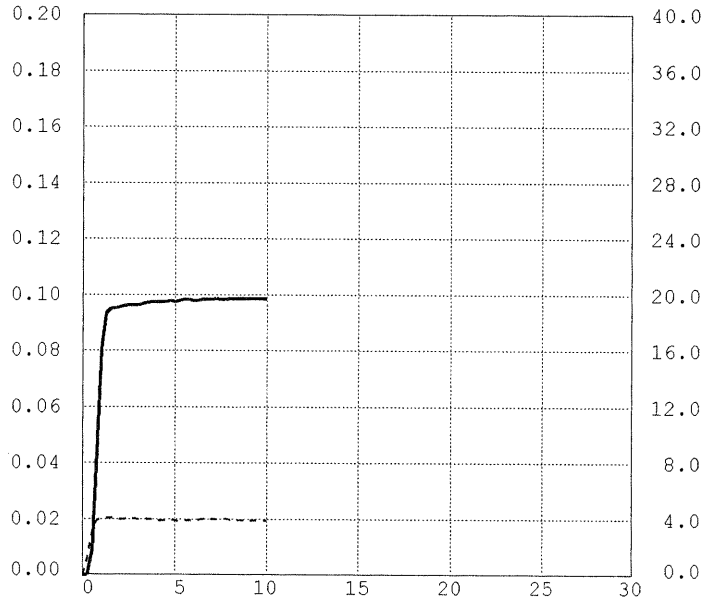

Charles B. Geisler #245