

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/02/2010

Operator Name: RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 09310

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:44
INTERNAL STANDARD	VERIFIED	02:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:44
BLANK TEST	0.00	02:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:45
BLANK TEST	0.00	02:46
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:46
BLANK TEST	0.00	02:47

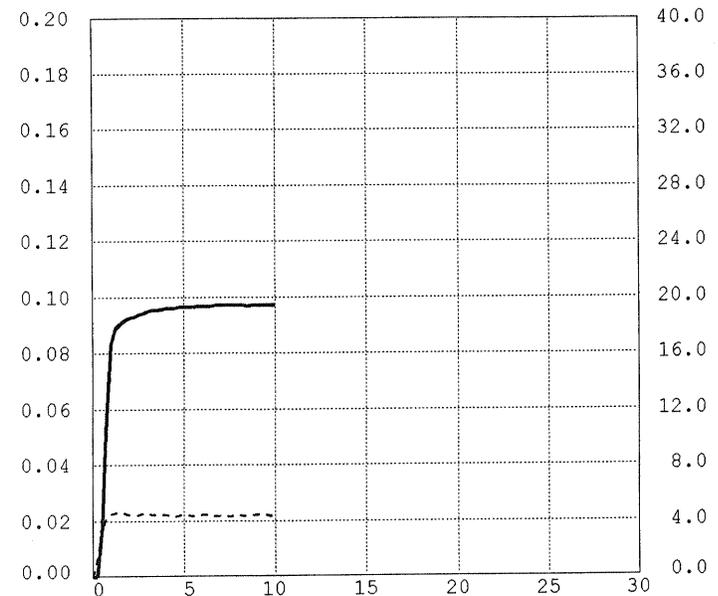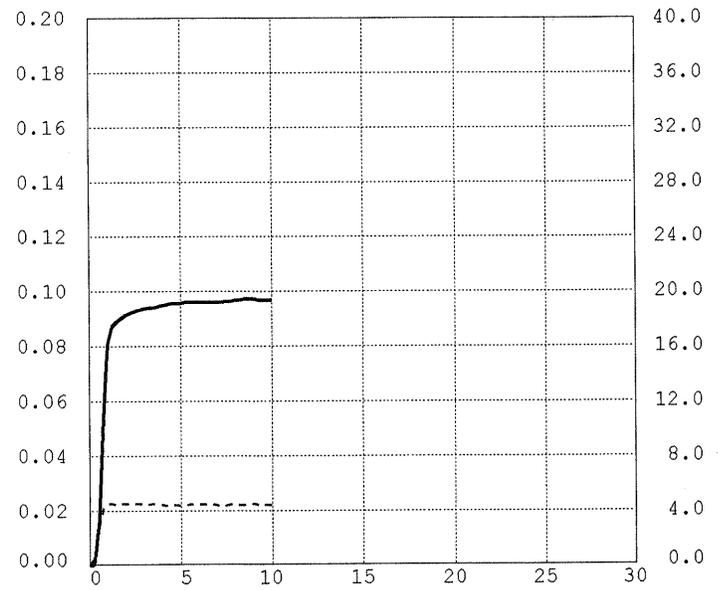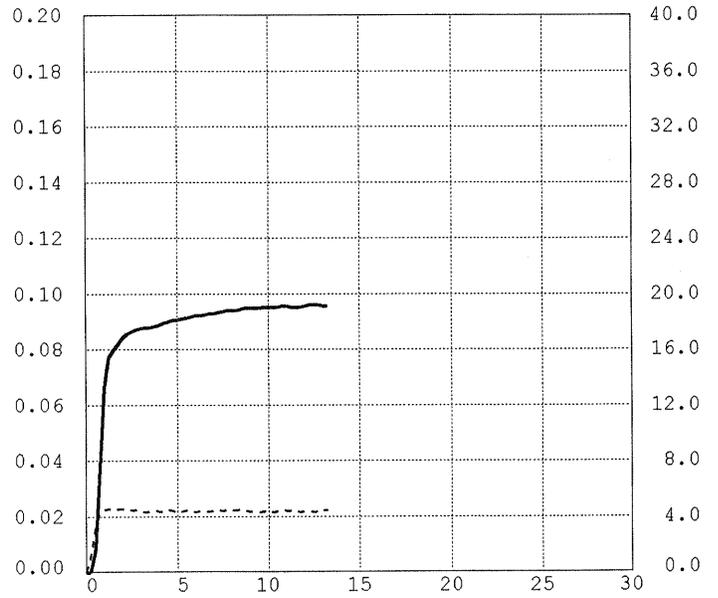

*SOB Ralph J Bartlett* WCSO SHF# 162 2-2-10