

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/08/2010

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 10010

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:20
INTERNAL STANDARD	VERIFIED	14:20
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	14:20
BLANK TEST	0.00	14:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	14:21
BLANK TEST	0.00	14:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:23
BLANK TEST	0.00	14:23

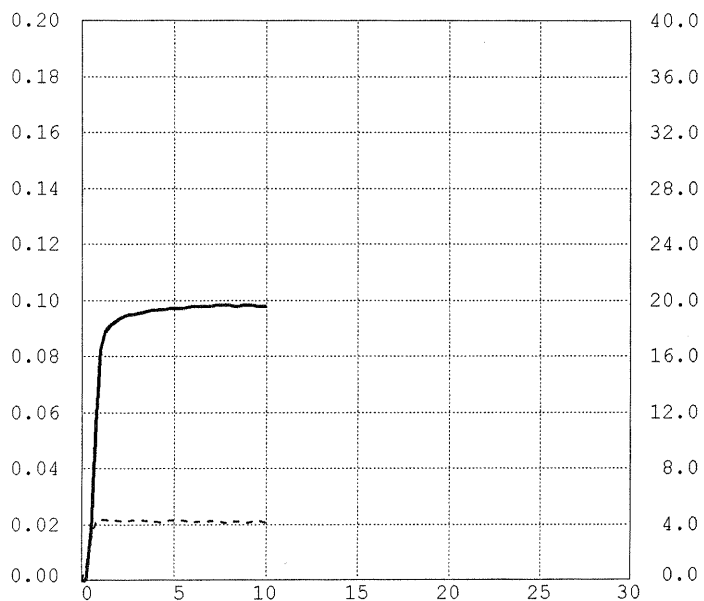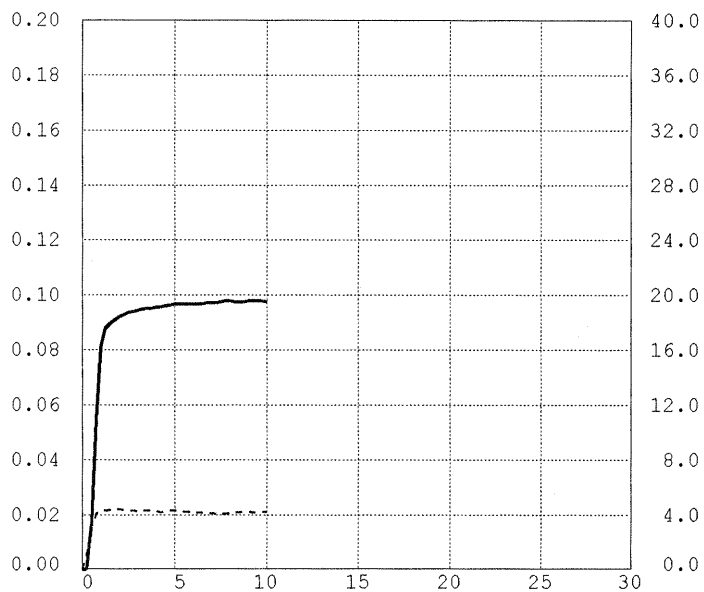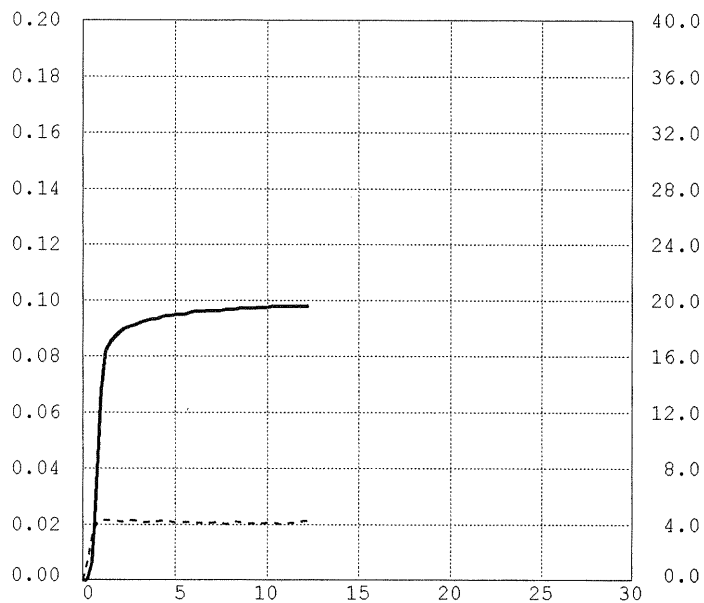

Charles B. Geisler #248