

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 05/27/2010

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 10010

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:20
INTERNAL STANDARD	VERIFIED	10:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:21
BLANK TEST	0.00	10:21
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	10:22
BLANK TEST	0.00	10:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:23
BLANK TEST	0.00	10:23

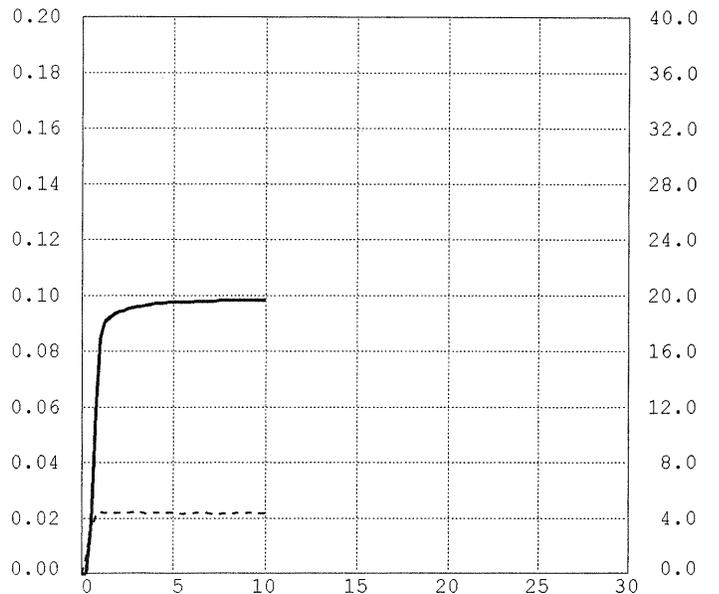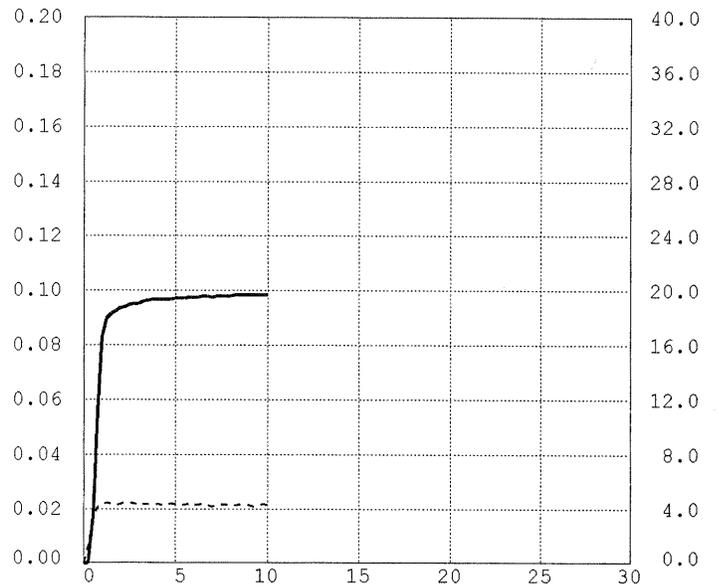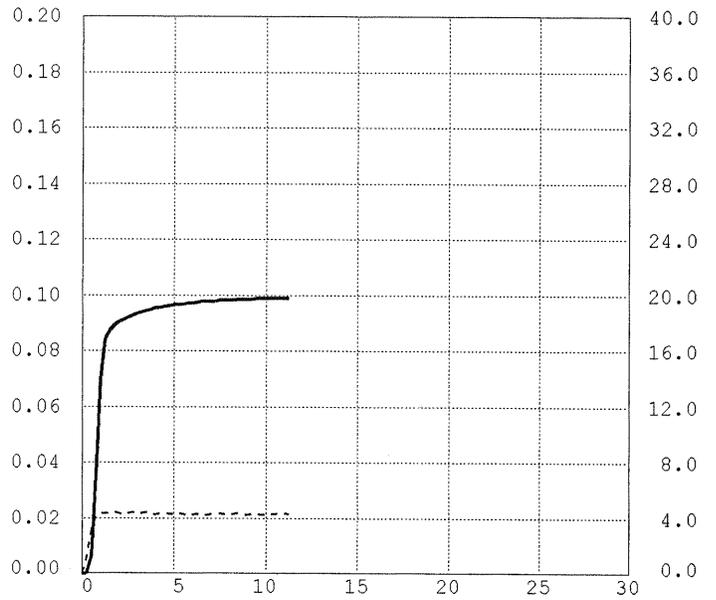

*Charles B. Geisler*