

SOLUTION CHANGE




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 06/01/2010

Operator Name: CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 10060

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:42
INTERNAL STANDARD	VERIFIED	11:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:42
BLANK TEST	0.00	11:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:43
BLANK TEST	0.00	11:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:44
BLANK TEST	0.00	11:45

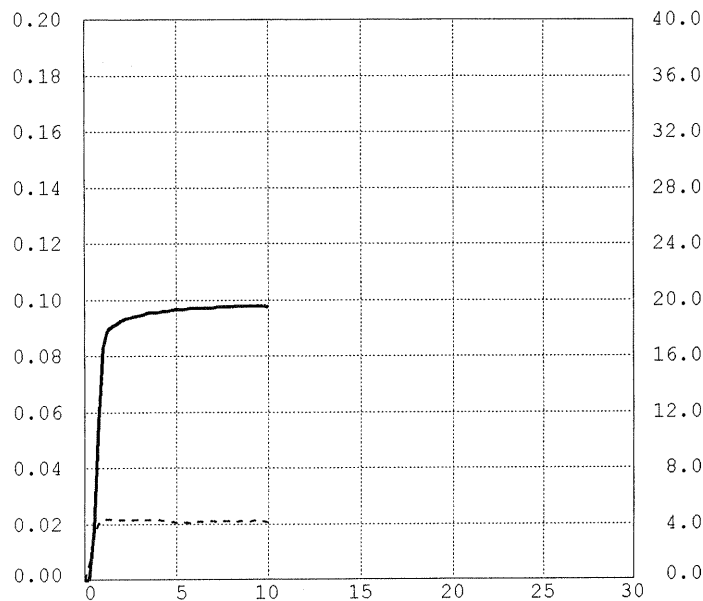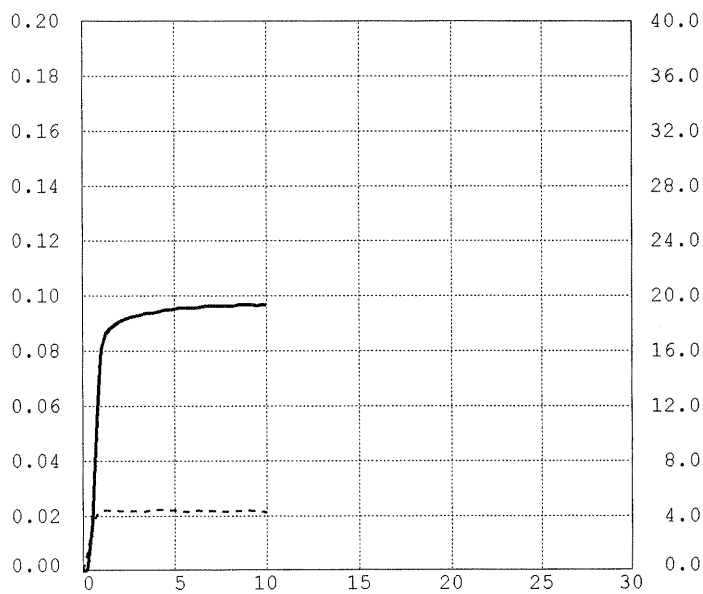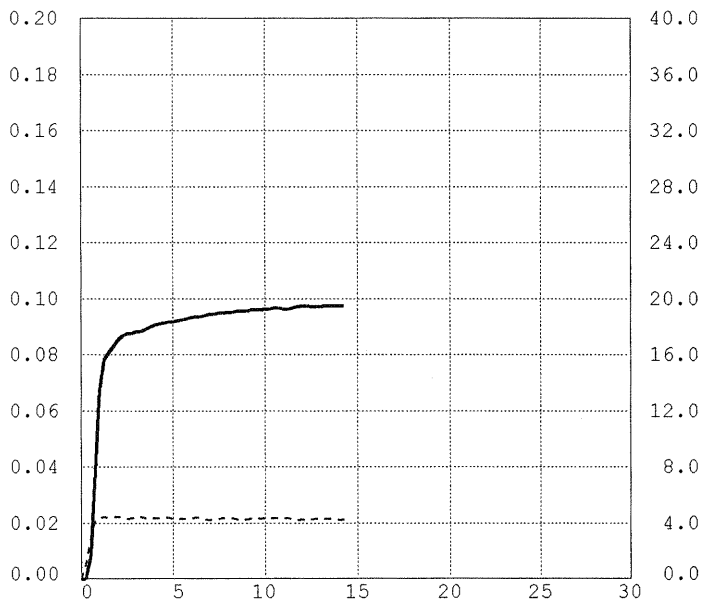

Charles B. Geisler
 #248 6/1/10 1149