

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 06/12/2010

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 10060

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:09
INTERNAL STANDARD	VERIFIED	15:09
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	15:09
BLANK TEST	0.00	15:10
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	15:10
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	15:11
BLANK TEST	0.00	15:12

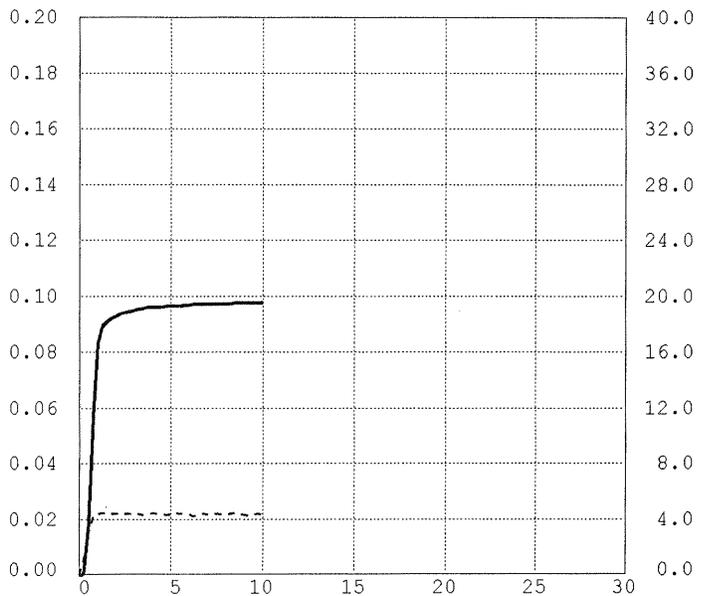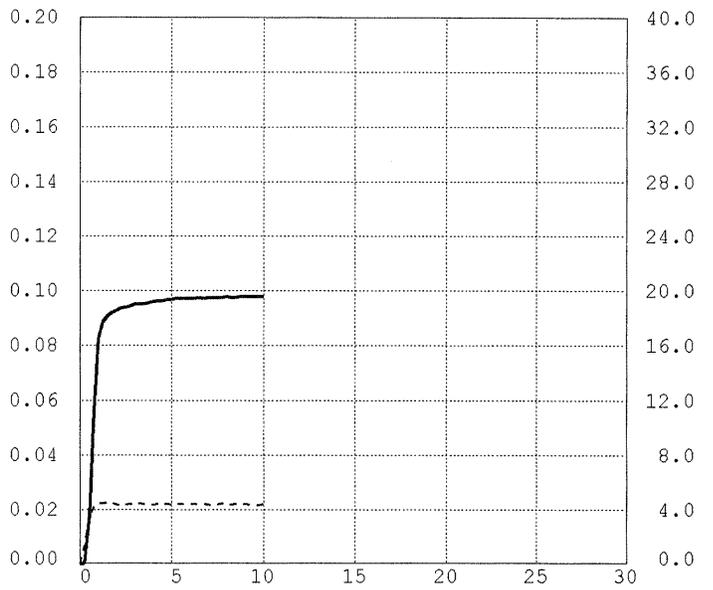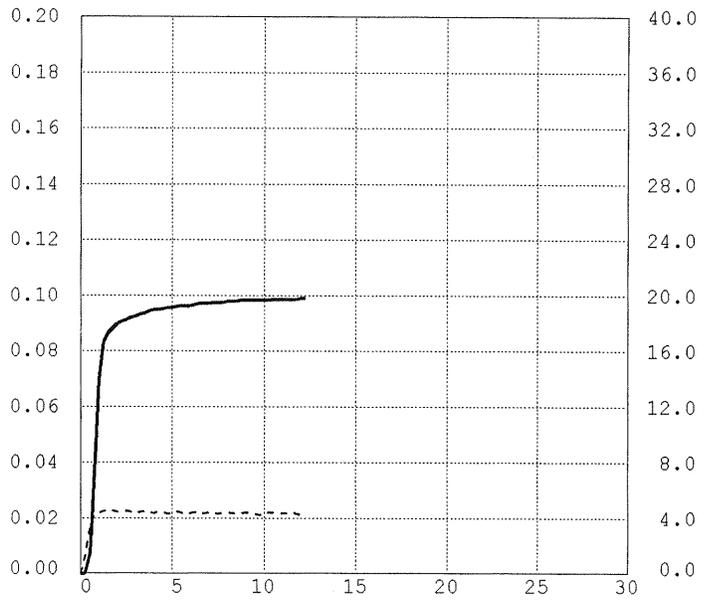

*Handwritten signature and notes:*  
#248 6/12/10 1516