

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/27/2010

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 10060

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:23
INTERNAL STANDARD	VERIFIED	15:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:24
BLANK TEST	0.00	15:24
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	15:25
BLANK TEST	0.00	15:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:26
BLANK TEST	0.00	15:27

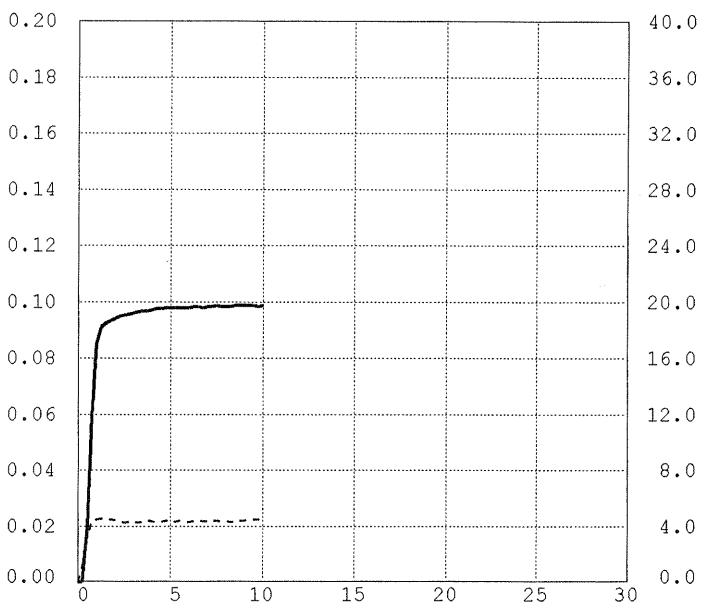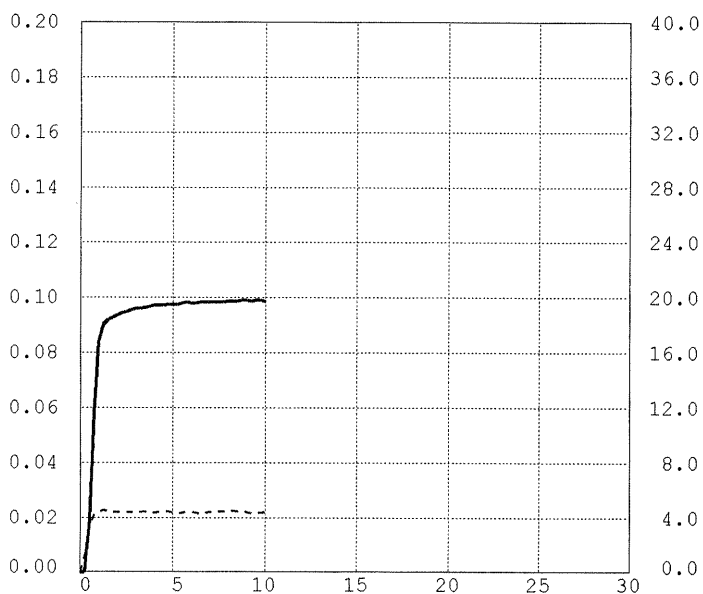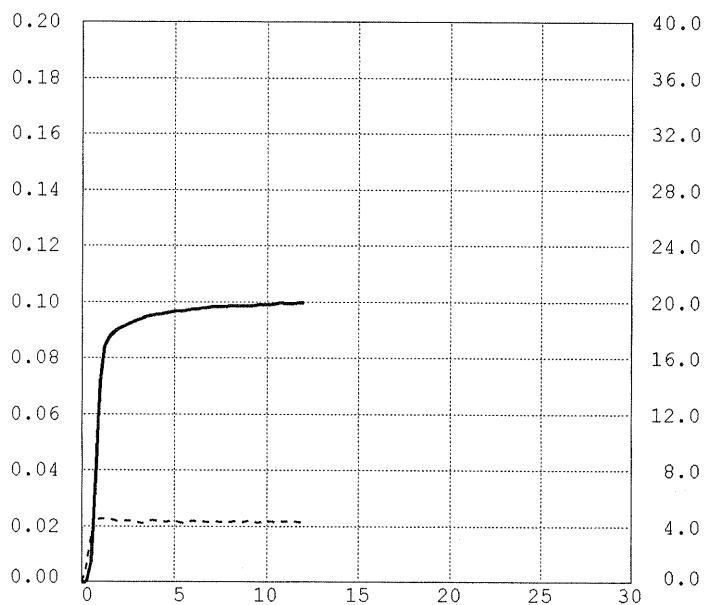

[Handwritten signature] #248 7/27/10
1532