

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 06/12/2010

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 10060

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:50
INTERNAL STANDARD	VERIFIED	14:50
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.10	14:50
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.10	14:51
REFERENCE STANDARD TEMP	34.0c	
REFERENCE STANDARD	0.10	14:52
BLANK TEST	0.00	14:53

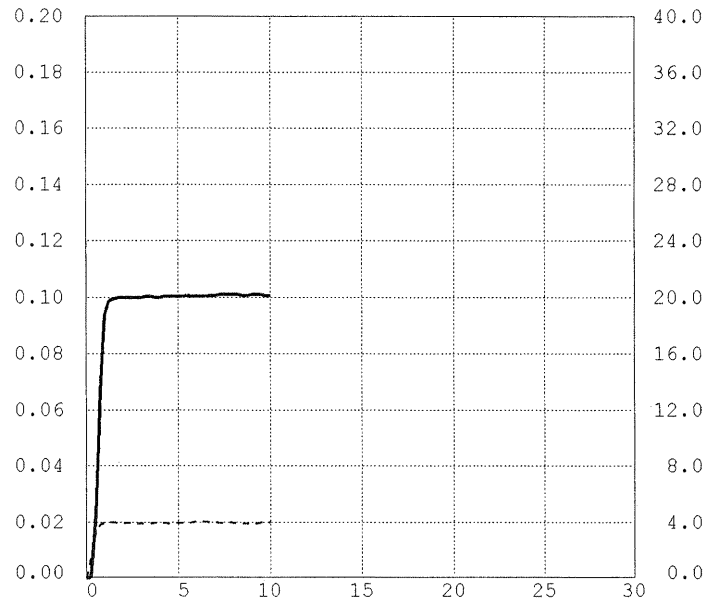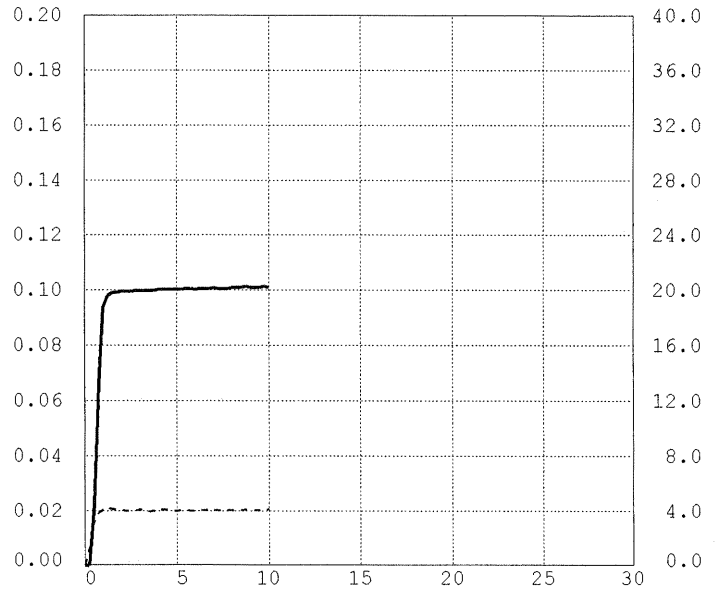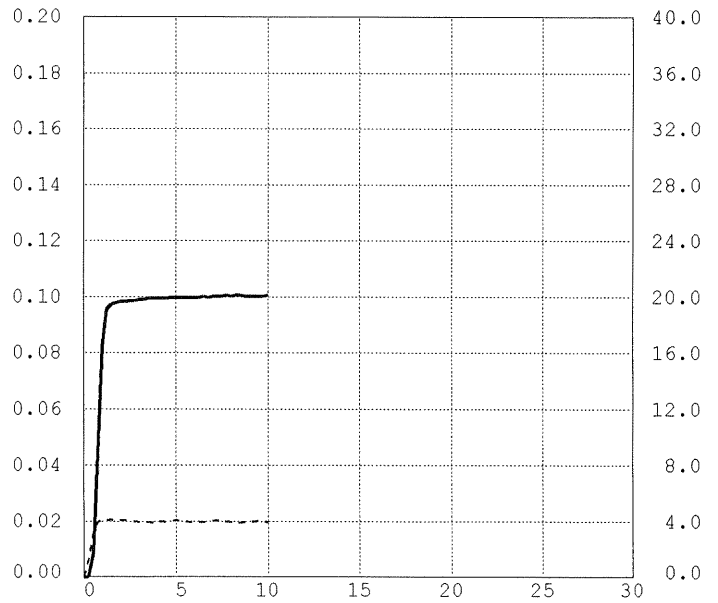

[Handwritten Signature]
#248 6/12/10 1453