

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 07/27/2010

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 10060

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:46
INTERNAL STANDARD	VERIFIED	15:46
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	15:46
BLANK TEST	0.00	15:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	15:47
BLANK TEST	0.00	15:48
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	15:48
BLANK TEST	0.00	15:49

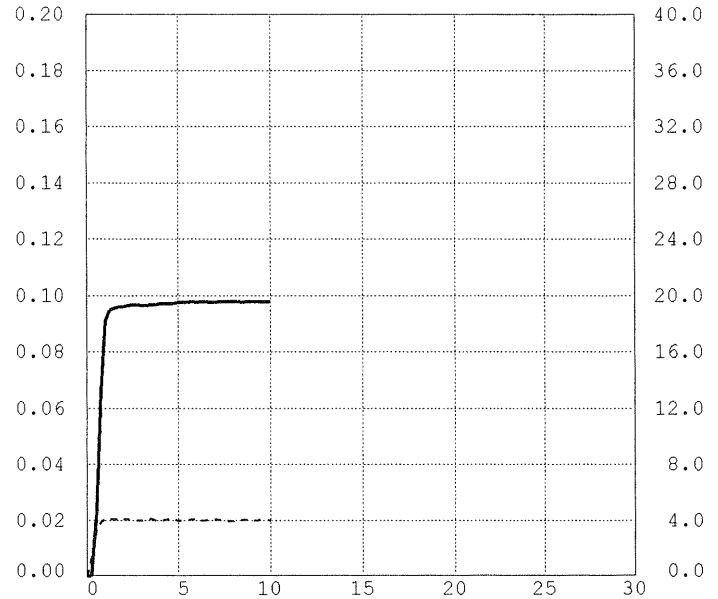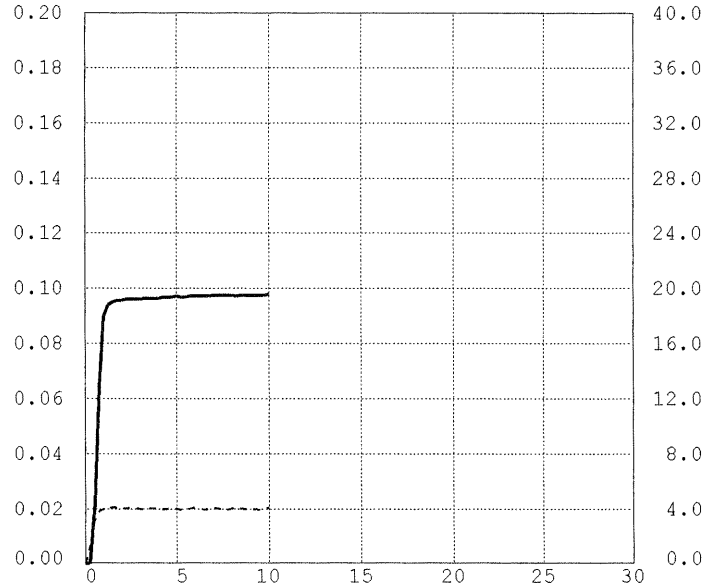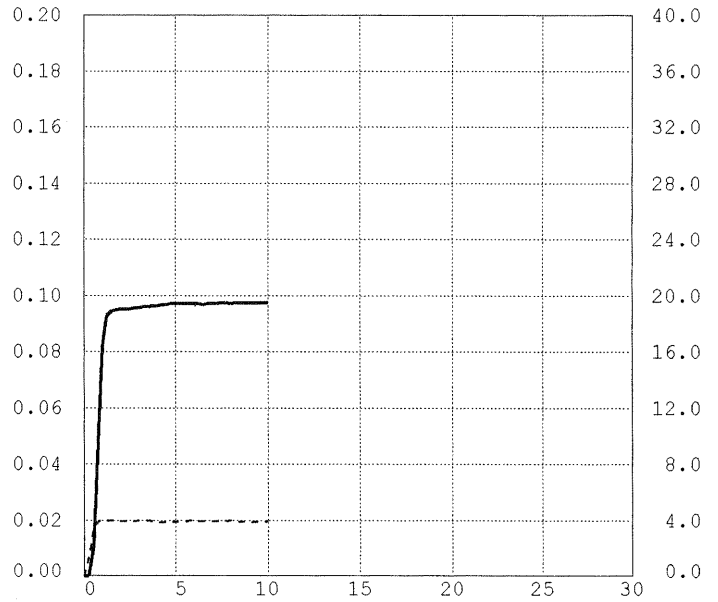

*Charles B. Geisler* #248 7/27/10  
1553