

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/16/2010

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 10140

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:09
INTERNAL STANDARD	VERIFIED	16:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	16:09
BLANK TEST	0.00	16:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	16:10
BLANK TEST	0.00	16:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	16:11
BLANK TEST	0.00	16:12

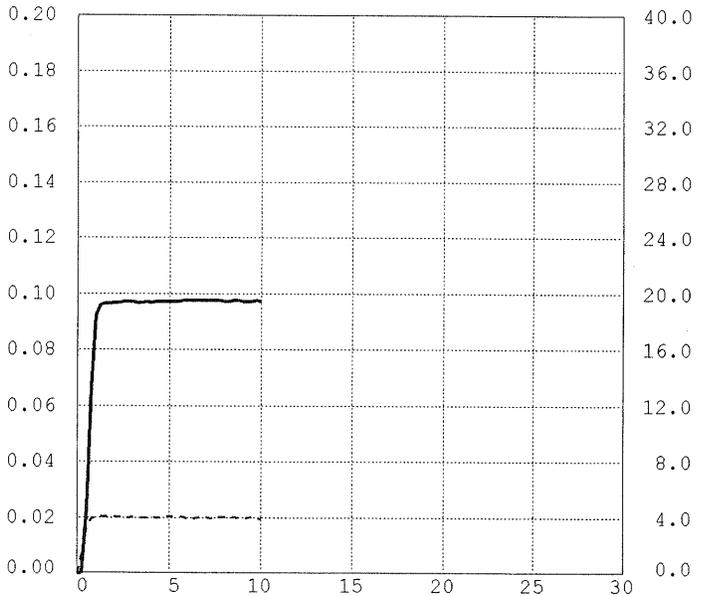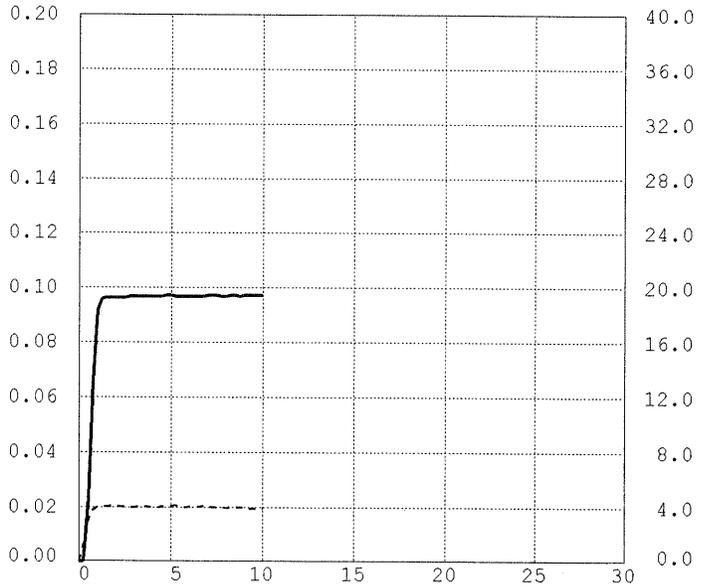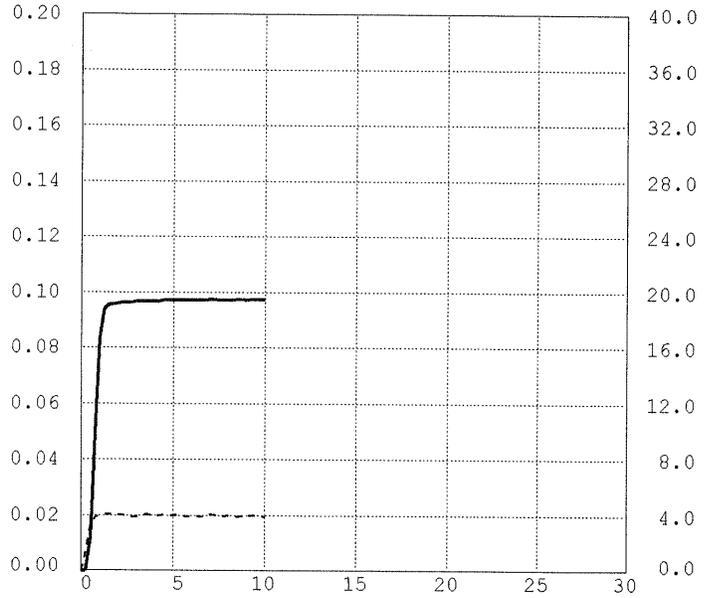

*Charles B. Geisler* #248