

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 11/23/2011

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 11140

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:12
INTERNAL STANDARD	VERIFIED	11:12
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:13
BLANK TEST	0.00	11:14
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:14
BLANK TEST	0.00	11:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:15
BLANK TEST	0.00	11:16

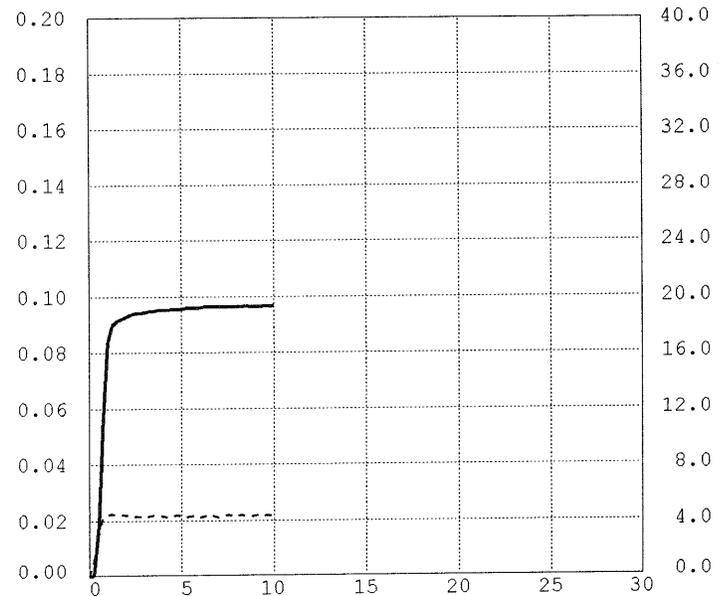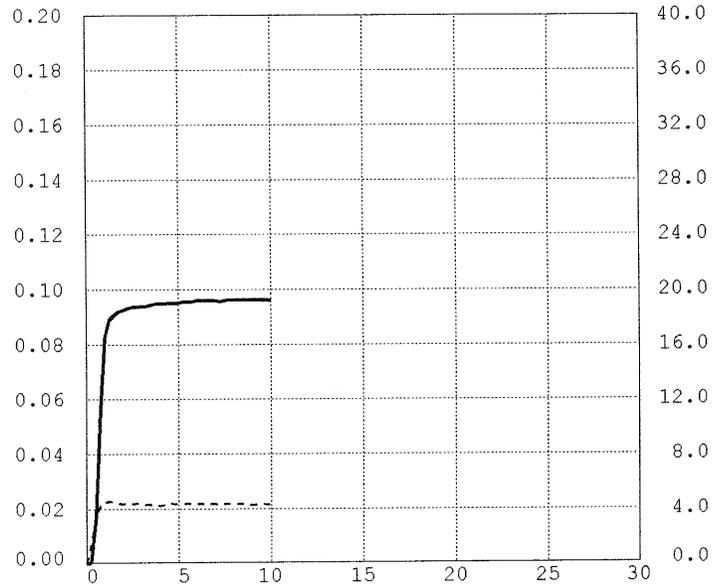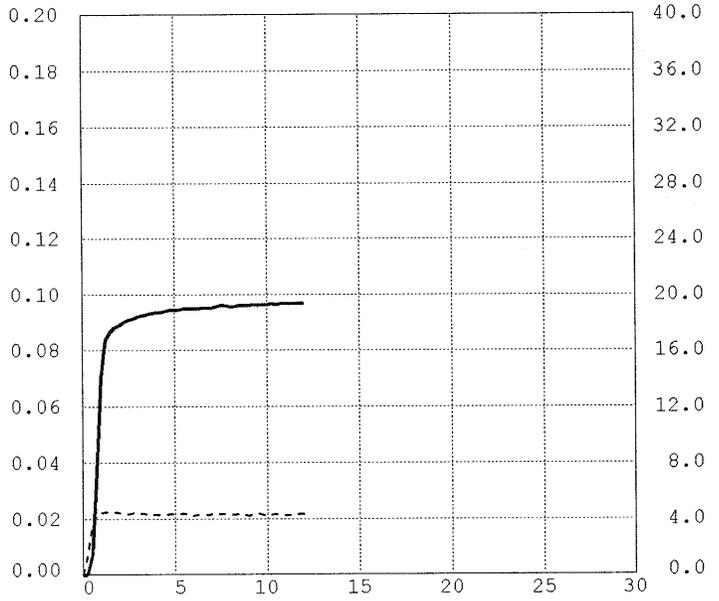

*Charles B. Geisler* #248 11/23/11 11:16 hours