

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 10/20/2011

Operator Name: RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 11140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:24
INTERNAL STANDARD	VERIFIED	01:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:24
BLANK TEST	0.00	01:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:25
BLANK TEST	0.00	01:26
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:26
BLANK TEST	0.00	01:27

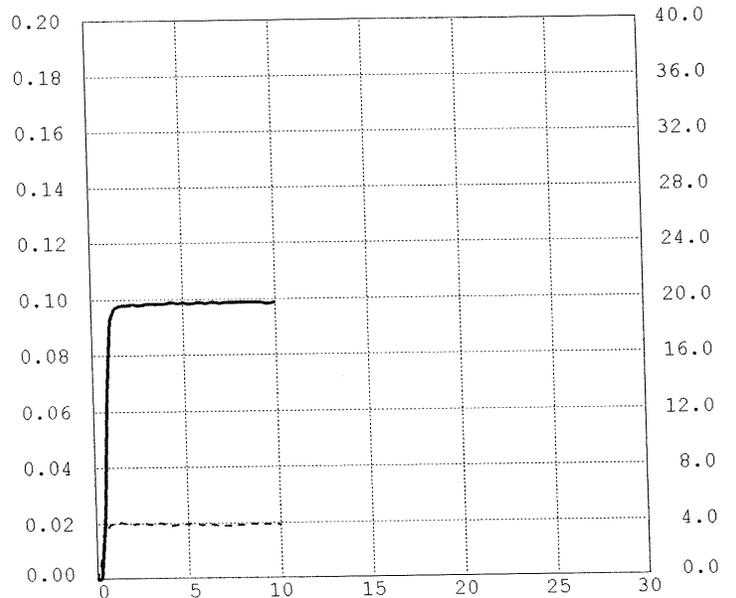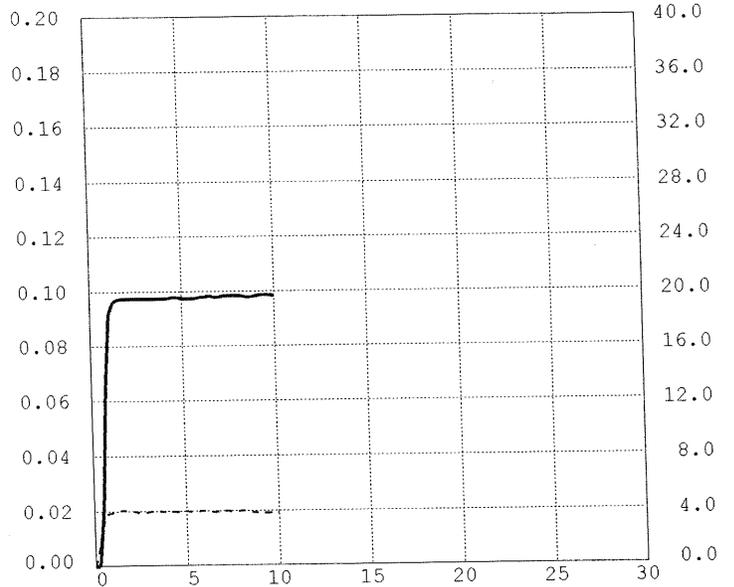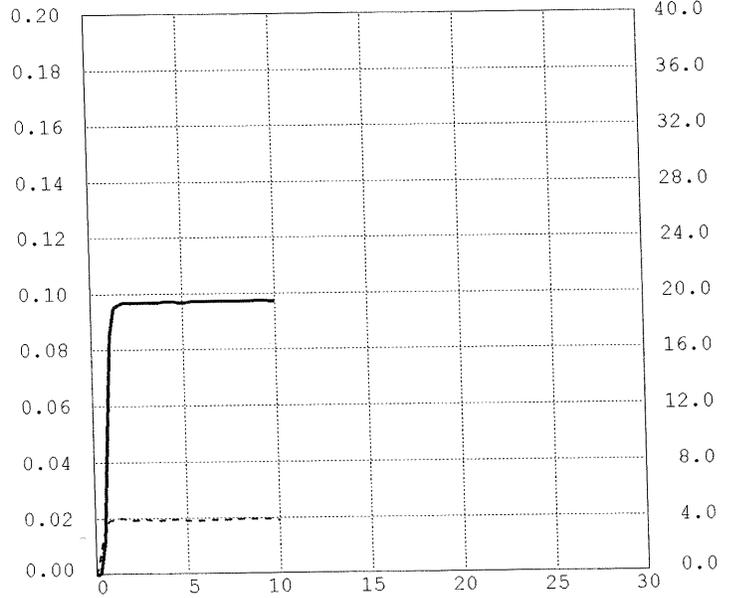

*[Handwritten scribbles and marks at the bottom of the page]*