

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/09/2011

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 11140

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:18
INTERNAL STANDARD	VERIFIED	12:18
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:18
BLANK TEST	0.00	12:19
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	12:19
BLANK TEST	0.00	12:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:20
BLANK TEST	0.00	12:21

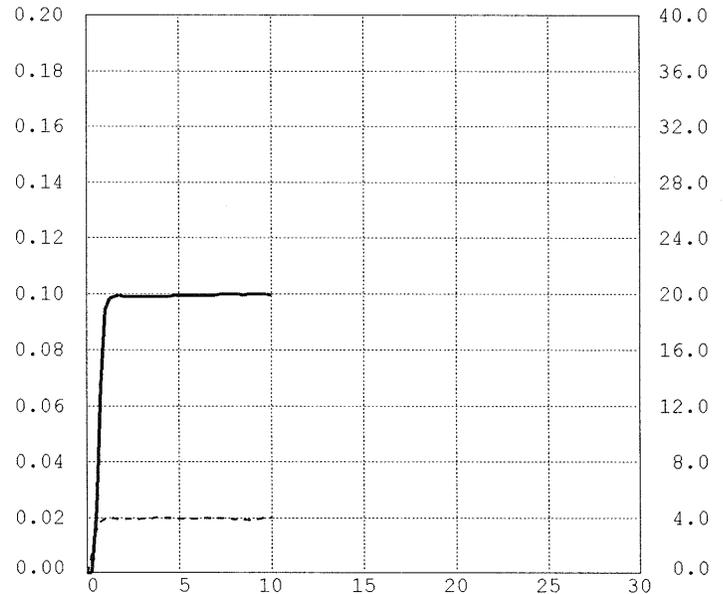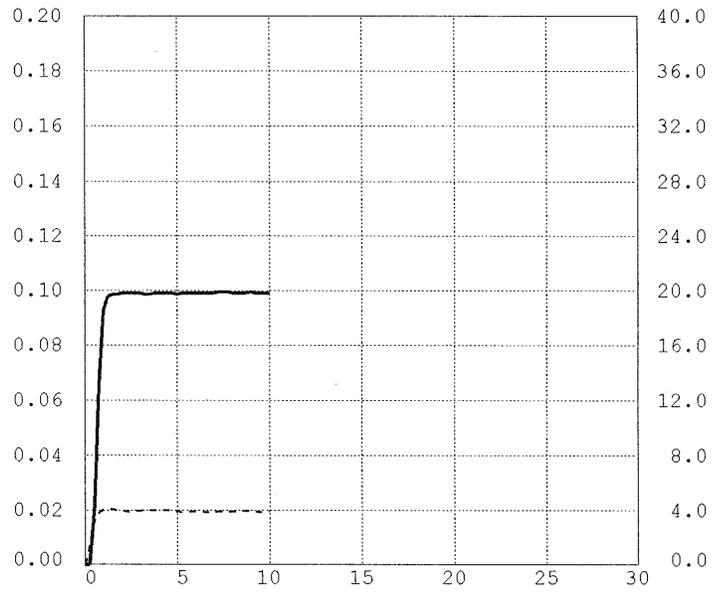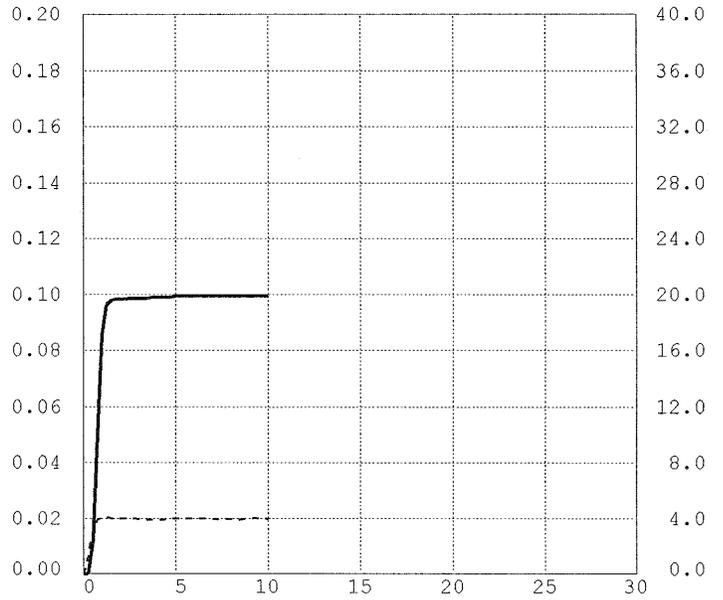

*for Chl B. J. #248 11/09/11 1221*