

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/15/2011

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 11140

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:36
INTERNAL STANDARD	VERIFIED	10:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:37
BLANK TEST	0.00	10:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:38
BLANK TEST	0.00	10:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:39
BLANK TEST	0.00	10:40

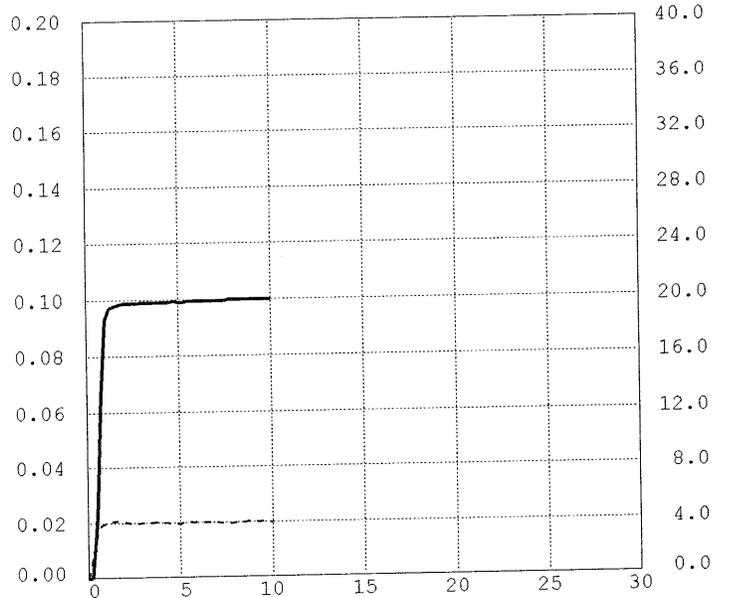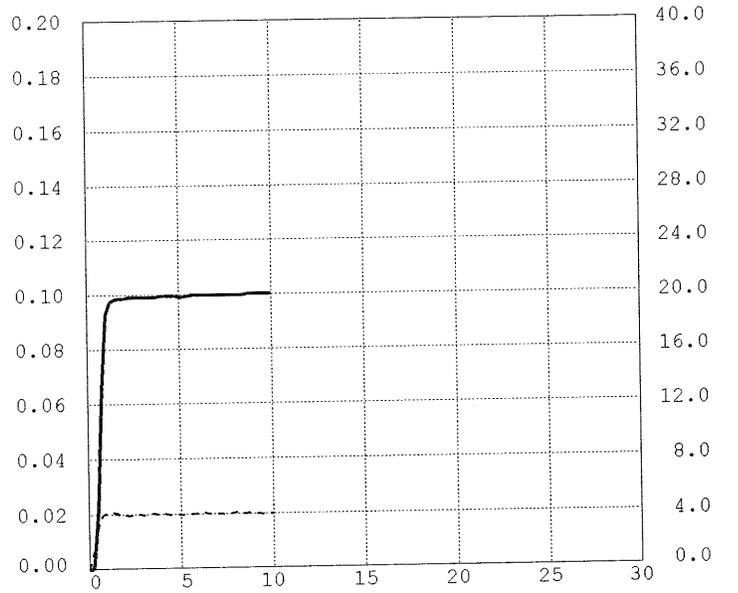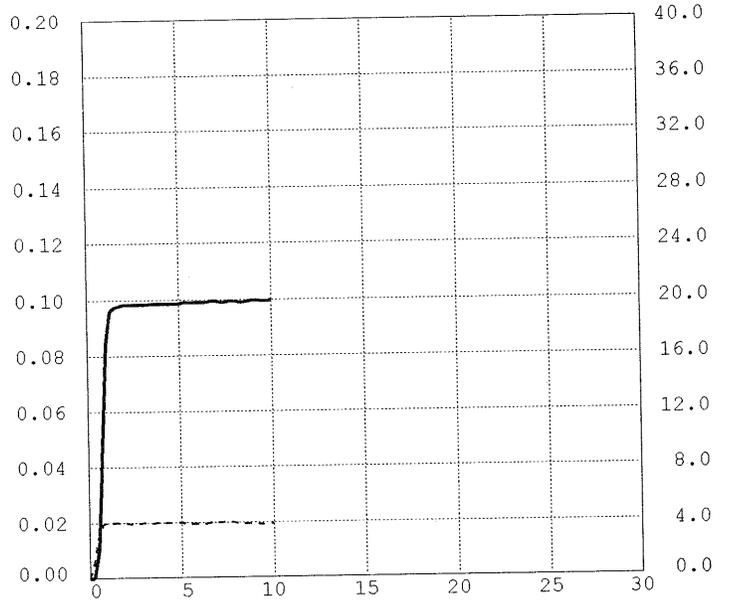

*for Mr. S. [Signature] #294 11/15/11 1040*