

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/23/2011

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 11140

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:39
INTERNAL STANDARD	VERIFIED	11:39
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:39
BLANK TEST	0.00	11:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:40
BLANK TEST	0.00	11:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:41
BLANK TEST	0.00	11:42

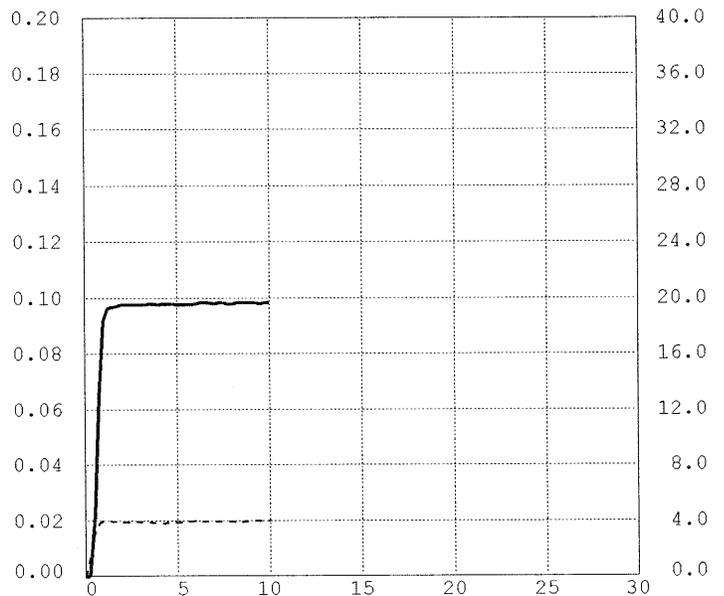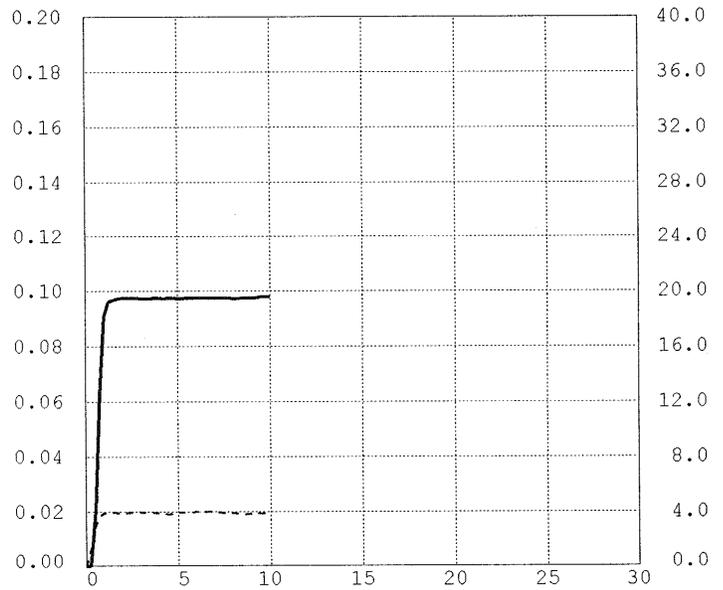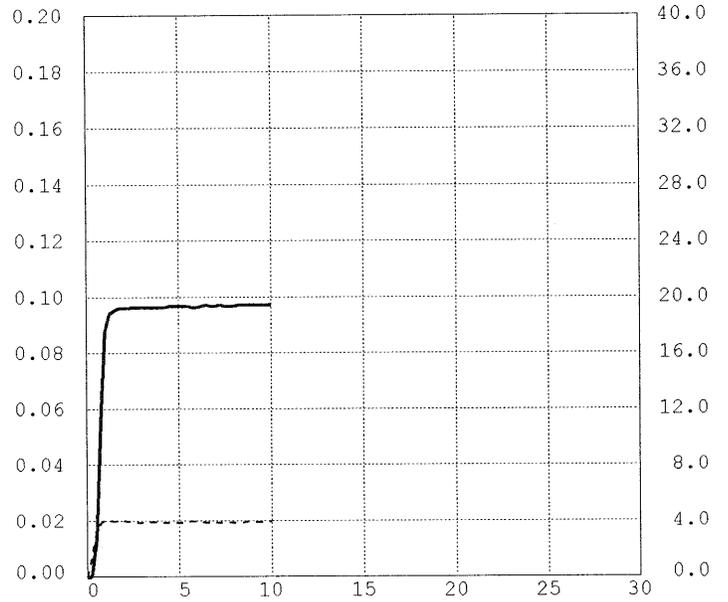

*Charles B. Geisler #240 11/23/11 11:42 AM*