

SUPERVISOR TEST




-----  
 WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208  
 -----

Date: 04/25/2012

Operator Name: RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 12020

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:33
INTERNAL STANDARD	VERIFIED	02:33
REFERENCE STANDARD TEMP	33.93c	
REFERENCE STANDARD	0.09	02:34
BLANK TEST	0.00	02:35
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	02:35
BLANK TEST	0.00	02:36
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:36
BLANK TEST	0.00	02:37

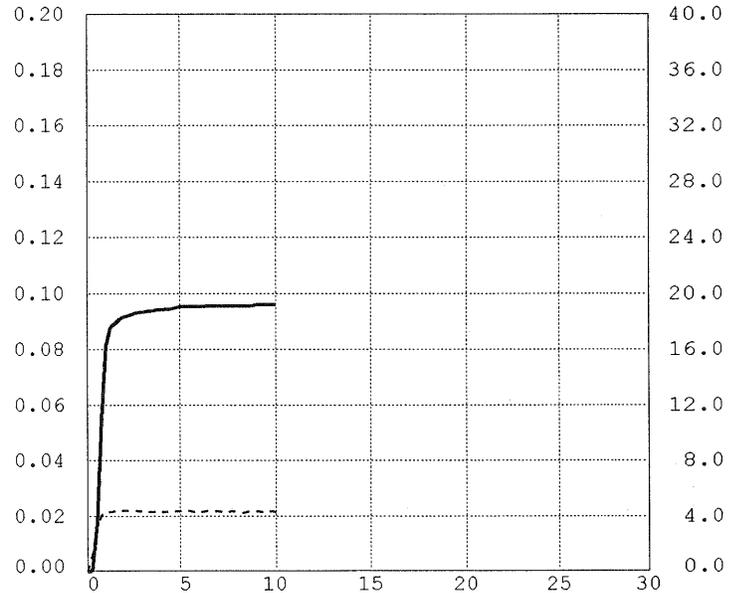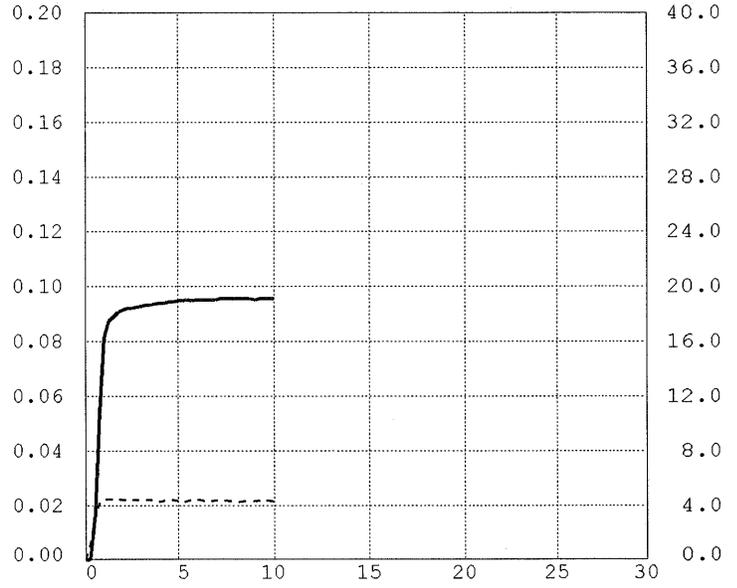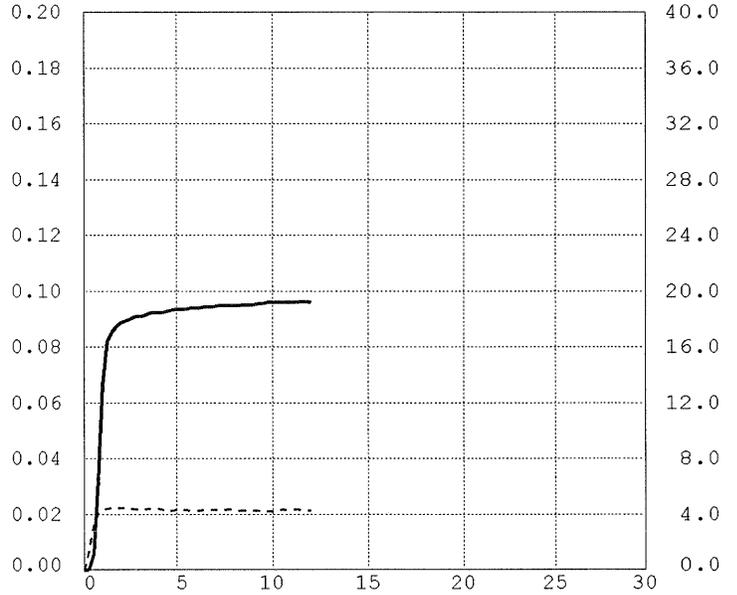

*R. J. Bartlett*      *04/25/12*