

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/07/2012

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 12110

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 09:28 |
| INTERNAL STANDARD | VERIFIED | 09:28 |
| REFERENCE STANDARD TEMP | 33.97c | |
| REFERENCE STANDARD | 0.09 | 09:28 |
| BLANK TEST | 0.00 | 09:29 |
| REFERENCE STANDARD TEMP | 33.97c | |
| REFERENCE STANDARD | 0.09 | 09:29 |
| BLANK TEST | 0.00 | 09:30 |
| REFERENCE STANDARD TEMP | 33.98c | |
| REFERENCE STANDARD | 0.09 | 09:30 |
| BLANK TEST | 0.00 | 09:31 |

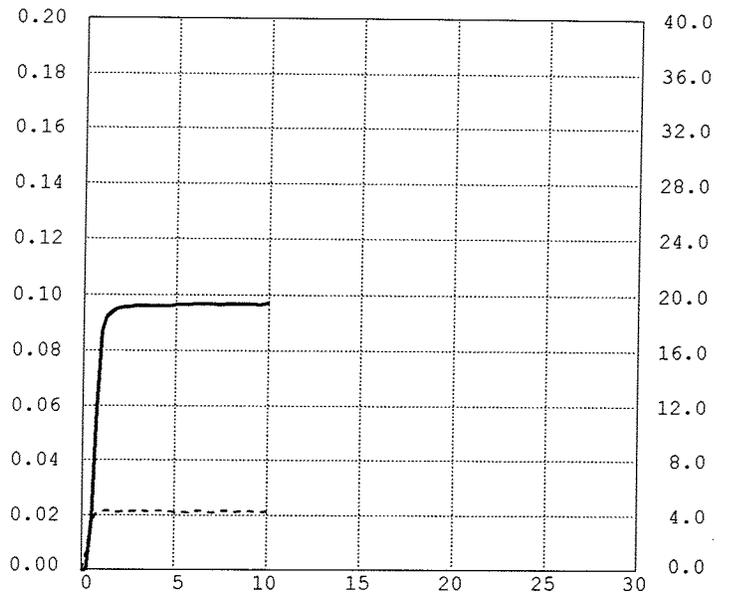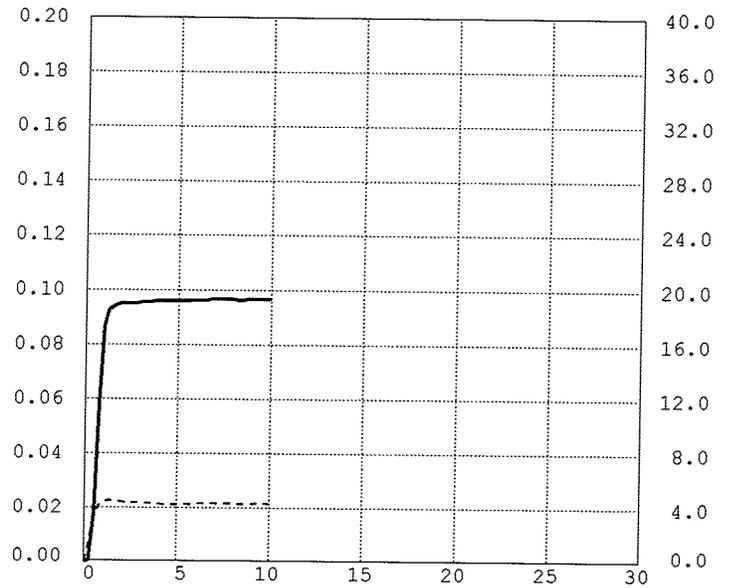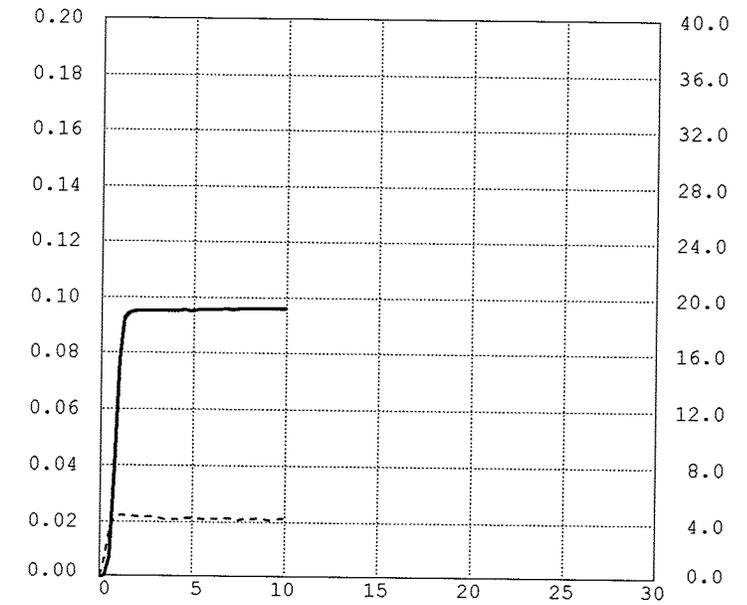

Charles B. Geisler #245