

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/01/2012

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 12190

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:45
INTERNAL STANDARD	VERIFIED	10:45
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	10:45
BLANK TEST	0.00	10:46
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	10:46
BLANK TEST	0.00	10:47
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	10:47
BLANK TEST	0.00	10:48

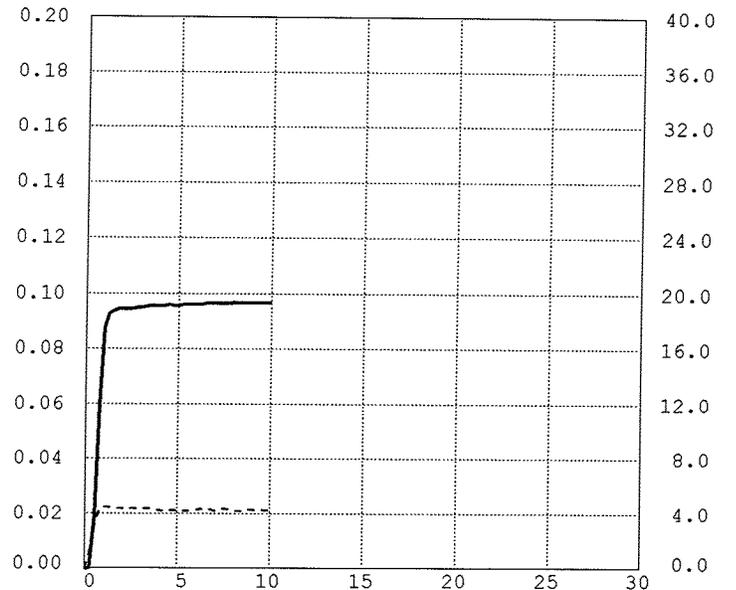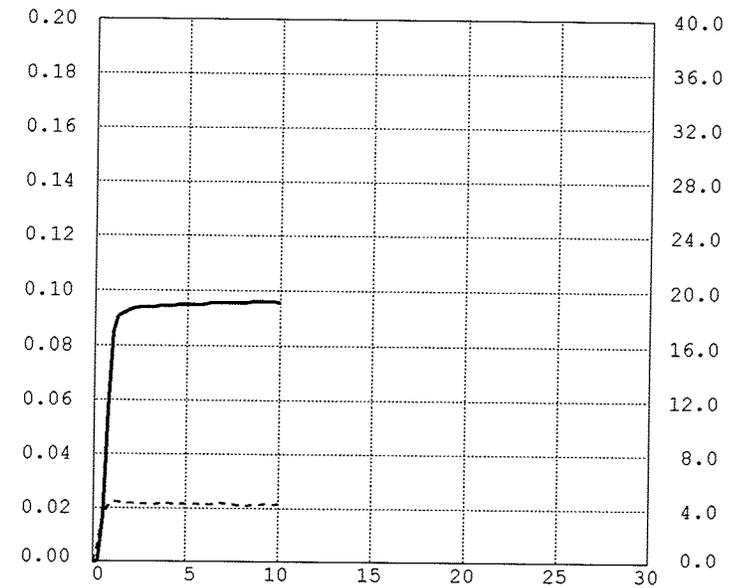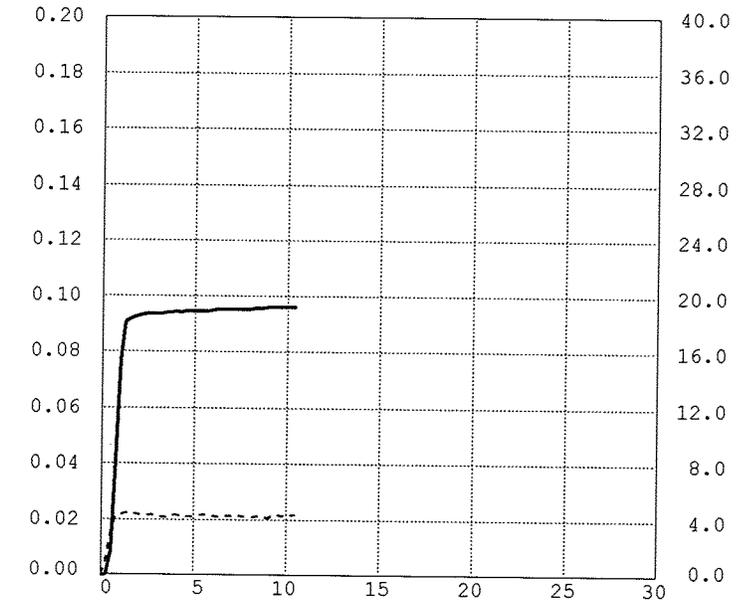

Charles B. Geisler #241