

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/01/2012

Operator Name: RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 12110

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:16
INTERNAL STANDARD	VERIFIED	01:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:16
BLANK TEST	0.00	01:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:17
BLANK TEST	0.00	01:18
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:18
BLANK TEST	0.00	01:19

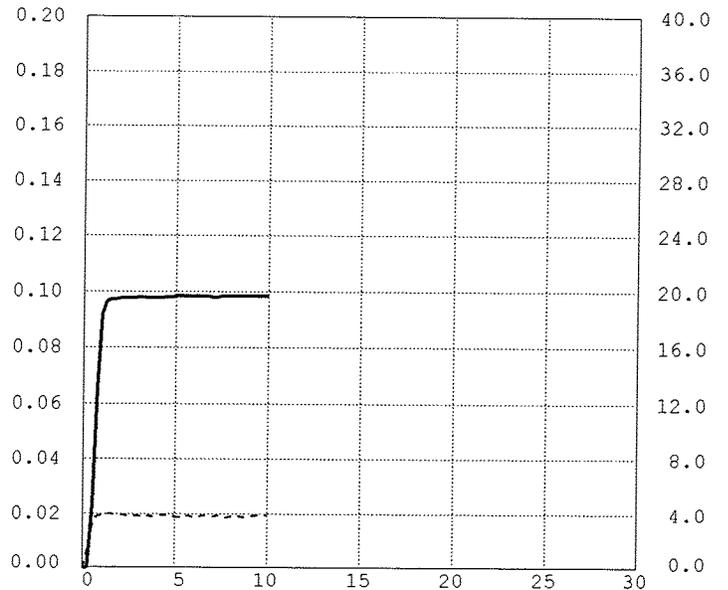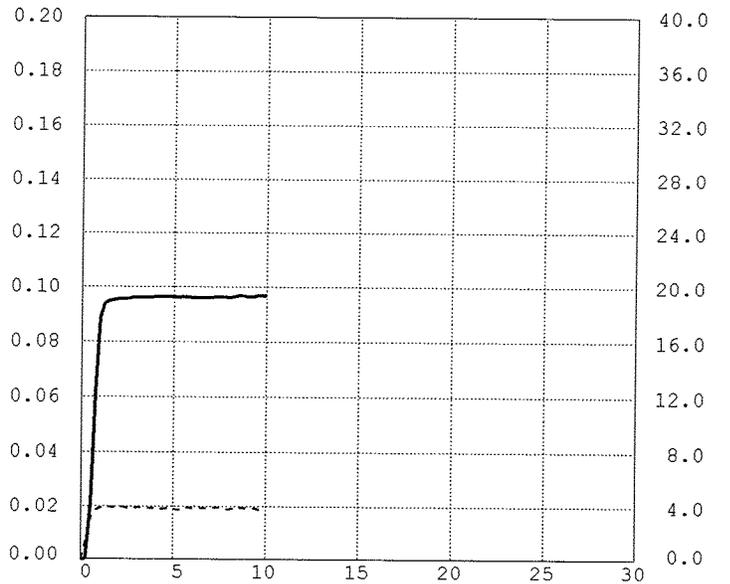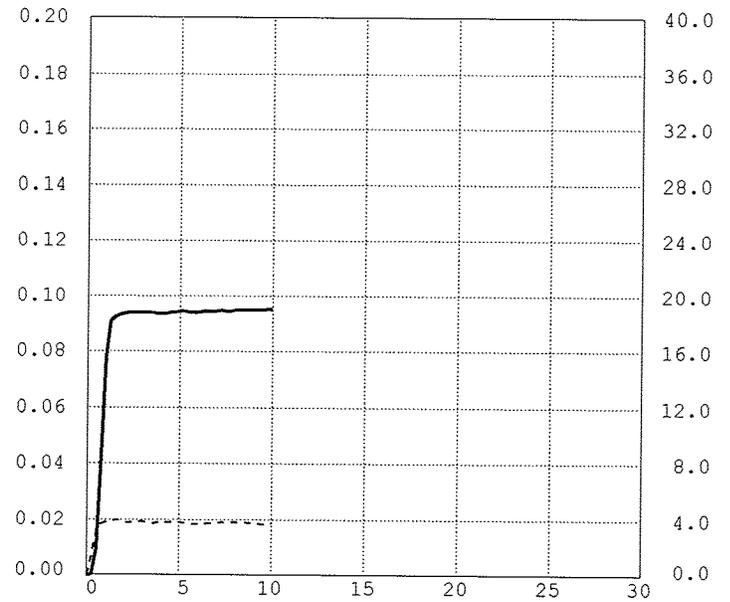

SG5 Run by [Signature]

WCSO #162 11-01-12