

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 11/07/2012

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 12110

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:00
INTERNAL STANDARD	VERIFIED	09:00
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	09:01
BLANK TEST	0.00	09:01
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	09:02
BLANK TEST	0.00	09:02
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:03
BLANK TEST	0.00	09:03

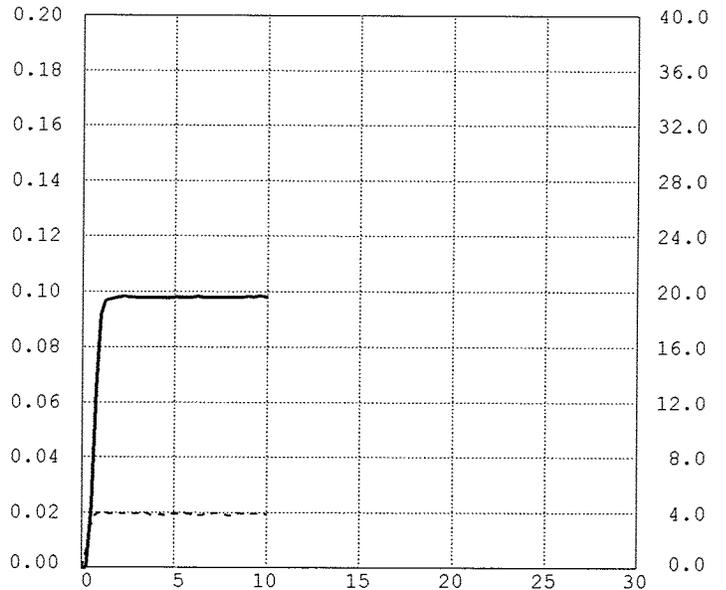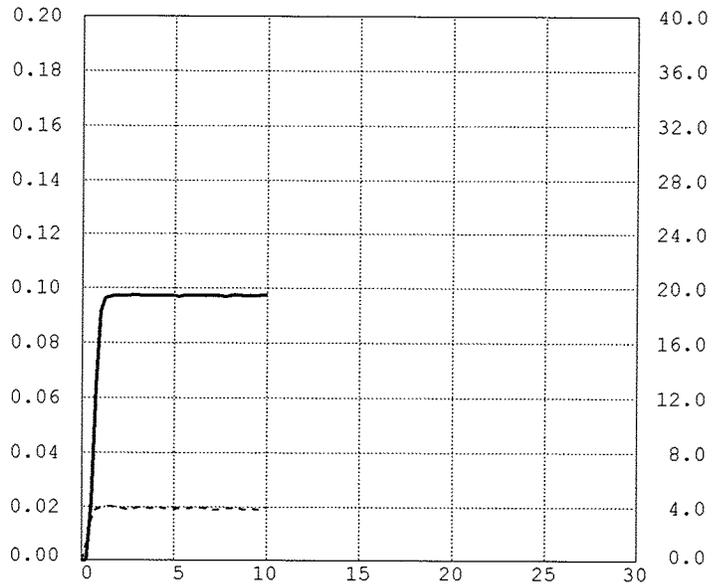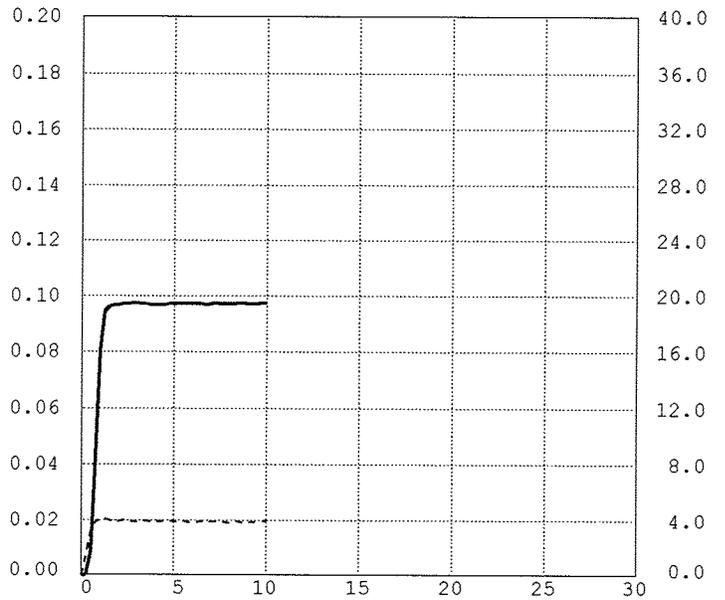

Charles B. Geisler #240