

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 11/13/2012

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 12110

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:49
INTERNAL STANDARD	VERIFIED	13:50
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	13:50
BLANK TEST	0.00	13:51
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	13:51
BLANK TEST	0.00	13:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:52
BLANK TEST	0.00	13:53

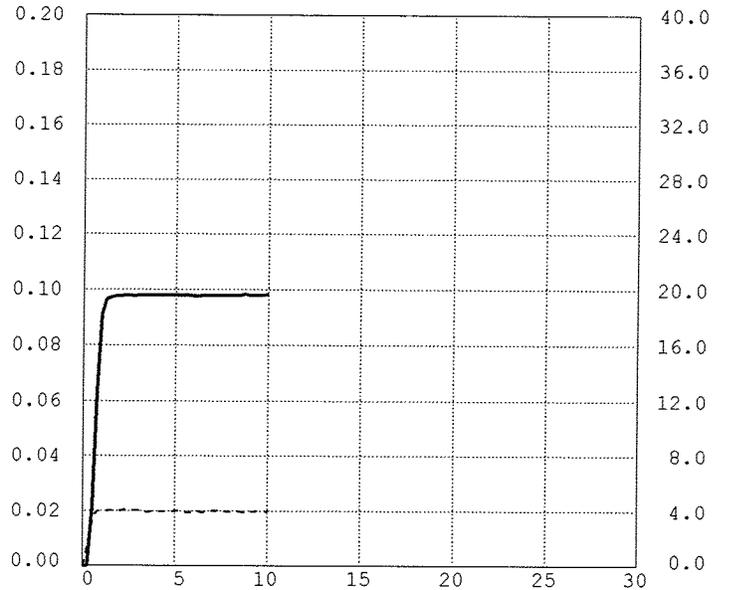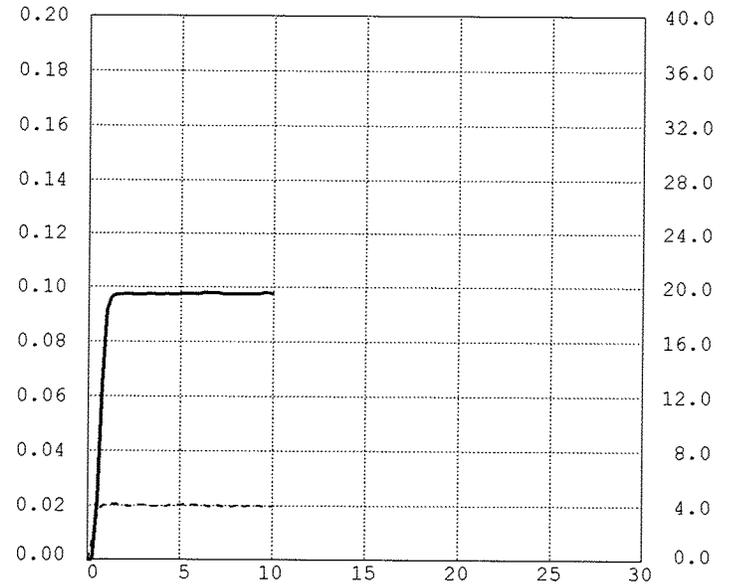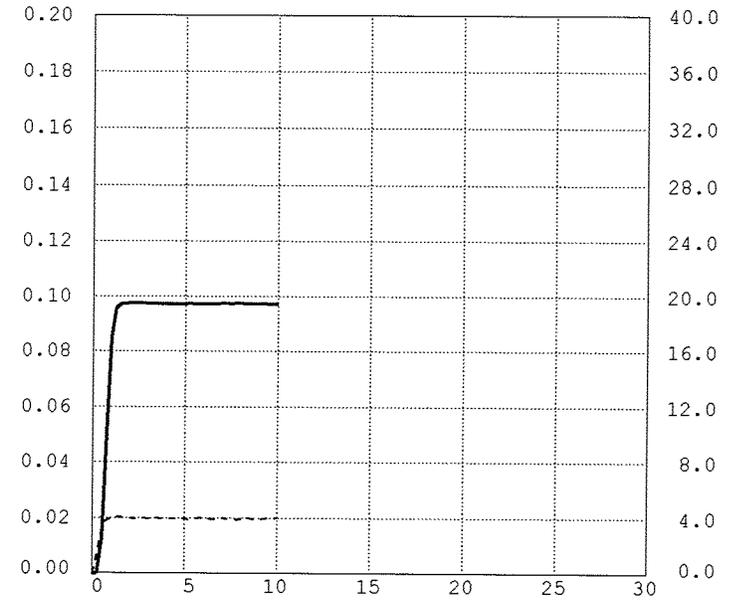

Charles B Geisler 11/13/12