

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 12/01/2012

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 12190

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:57
INTERNAL STANDARD	VERIFIED	09:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:57
BLANK TEST	0.00	09:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:58
BLANK TEST	0.00	09:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:59
BLANK TEST	0.00	10:00

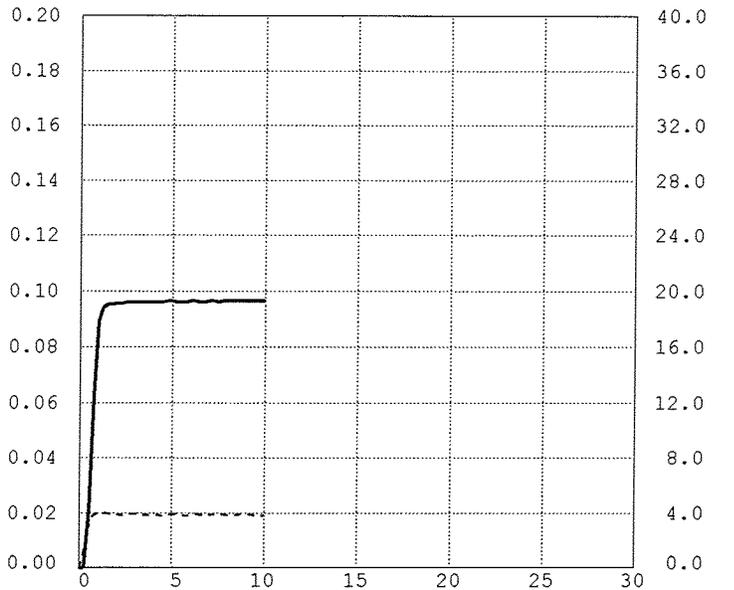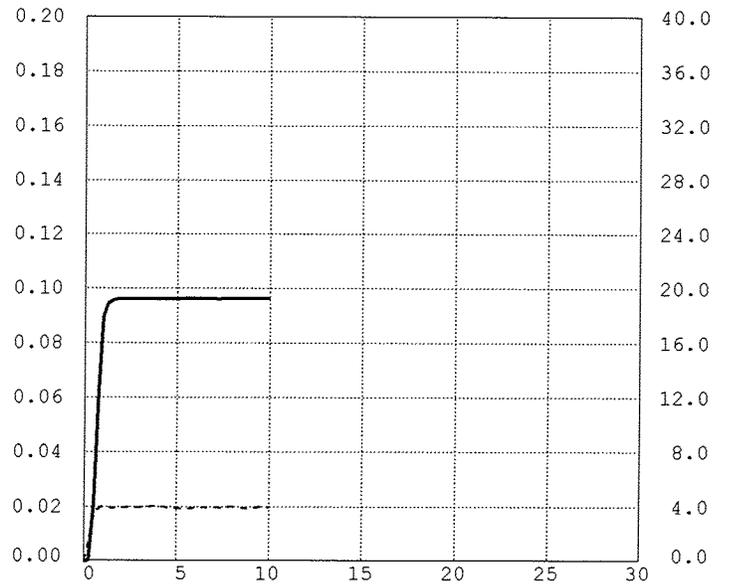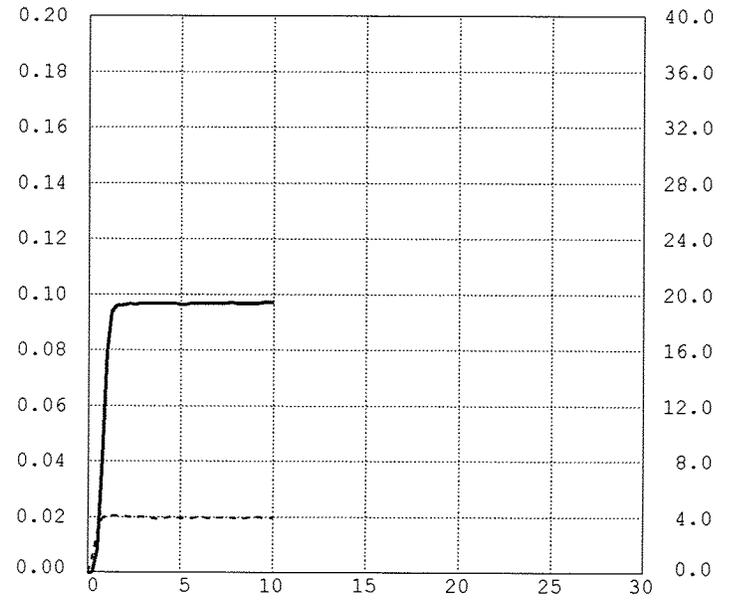

A. C. B. [Signature] #244