

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/17/2013

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13200

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:54
INTERNAL STANDARD	VERIFIED	09:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	09:54
BLANK TEST	0.00	09:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:55
BLANK TEST	0.00	09:56
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	09:56
BLANK TEST	0.00	09:57

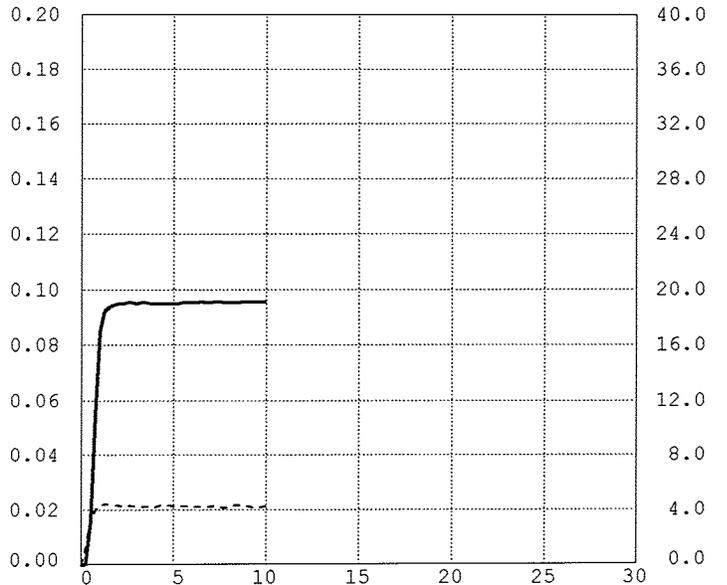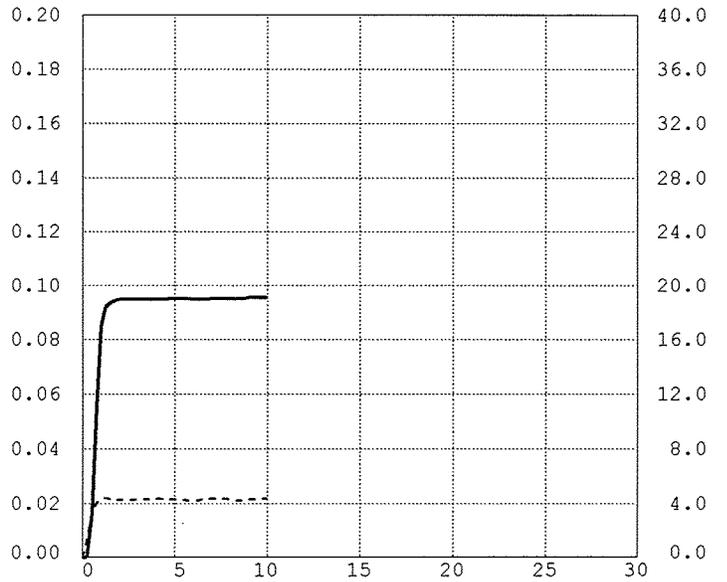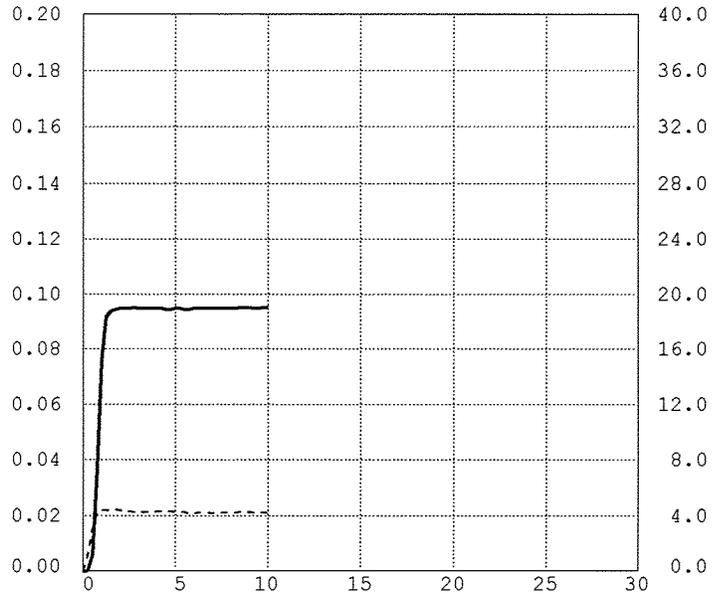

J. M. B. #248 11/17/13
3000