

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/01/2013

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13260

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:35
INTERNAL STANDARD	VERIFIED	10:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:35
BLANK TEST	0.00	10:36
REFERENCE STANDARD TEMP	33.94c	
REFERENCE STANDARD	0.09	10:36
BLANK TEST	0.00	10:37
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	10:37
BLANK TEST	0.00	10:38

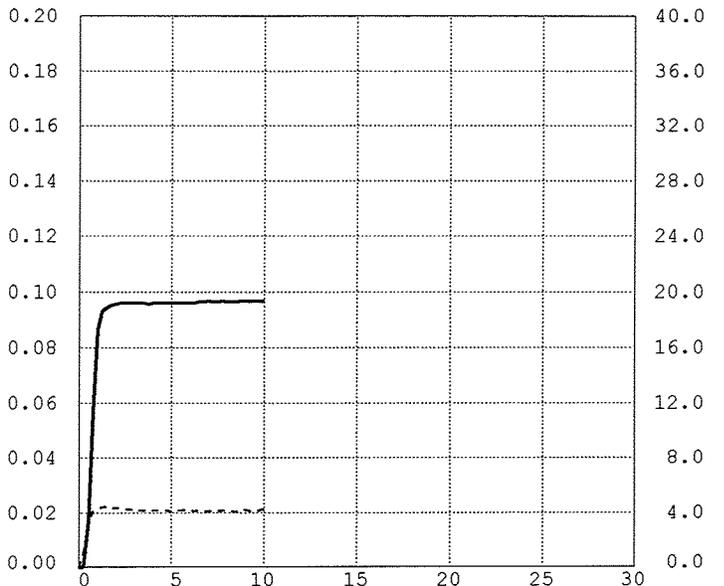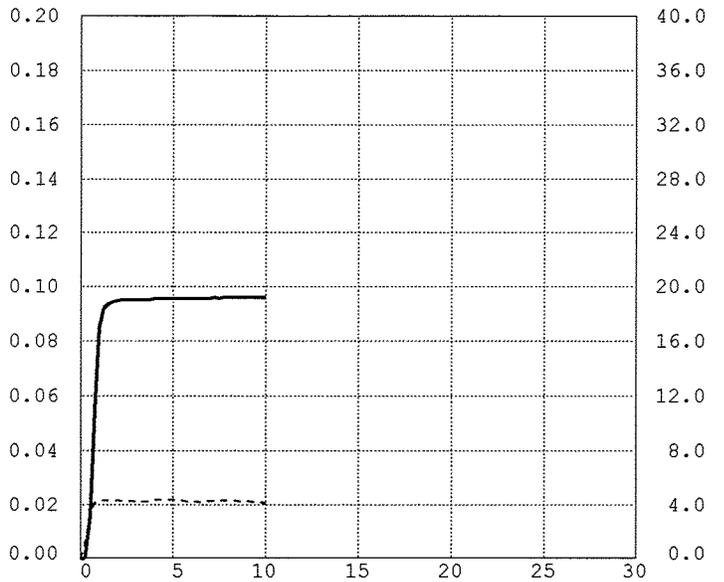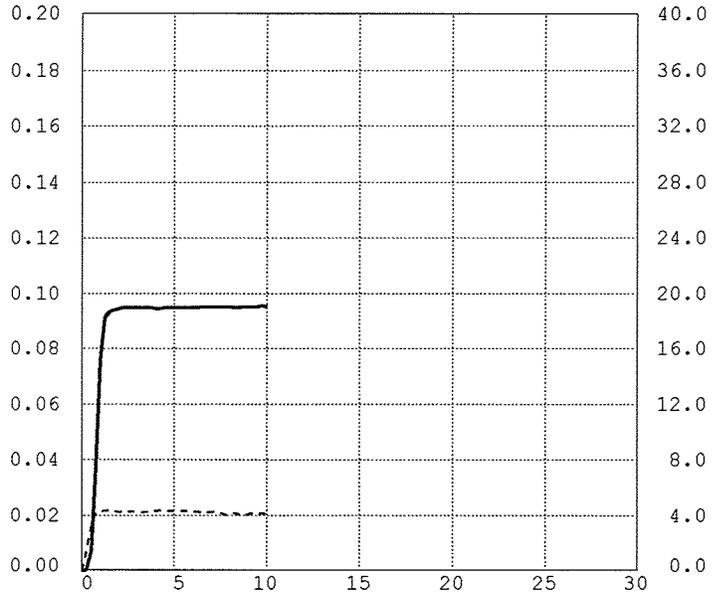

Charles B. Geisler
#245 12/01/13
1041