

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 08/19/2013

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13140

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:10
INTERNAL STANDARD	VERIFIED	19:10
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	19:10
BLANK TEST	0.00	19:11
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	19:12
BLANK TEST	0.00	19:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:13
BLANK TEST	0.00	19:13

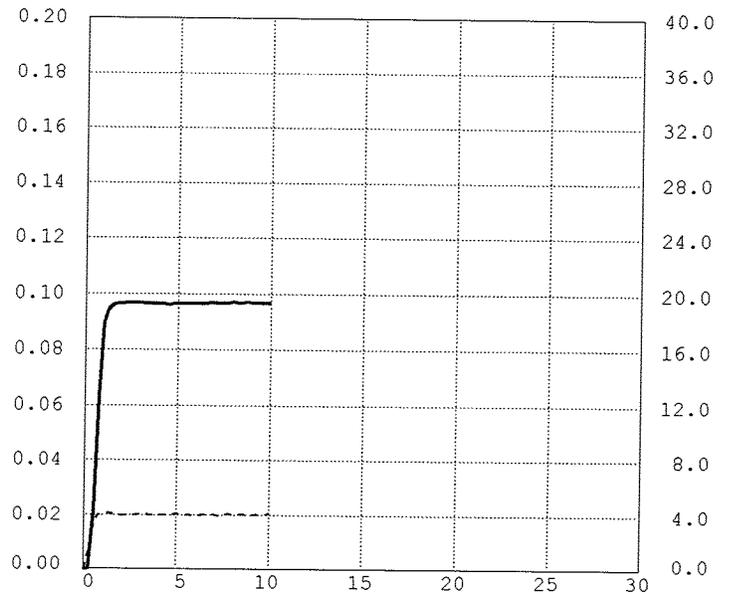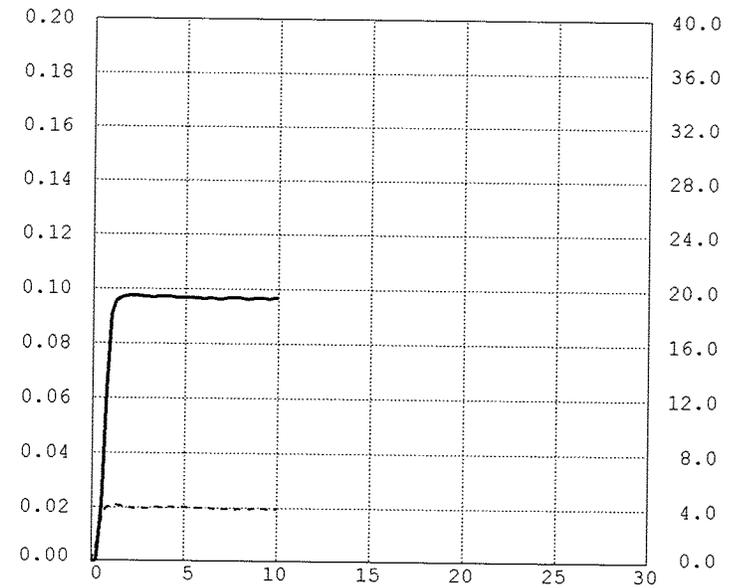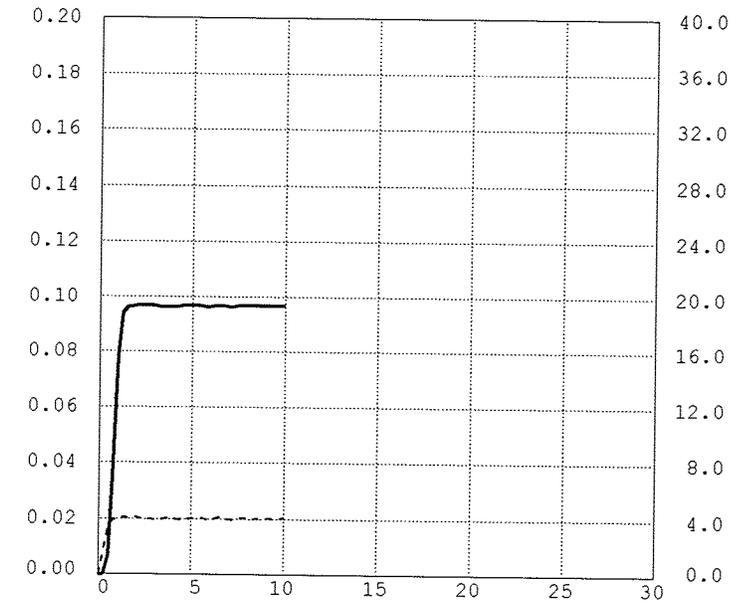

Charles B Geisler
#246