

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 144506

Date: 09/24/2013

Operator Name: RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 13140

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:56
INTERNAL STANDARD	VERIFIED	00:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:56
BLANK TEST	0.00	00:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:57
BLANK TEST	0.00	00:58
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:58
BLANK TEST	0.00	00:59

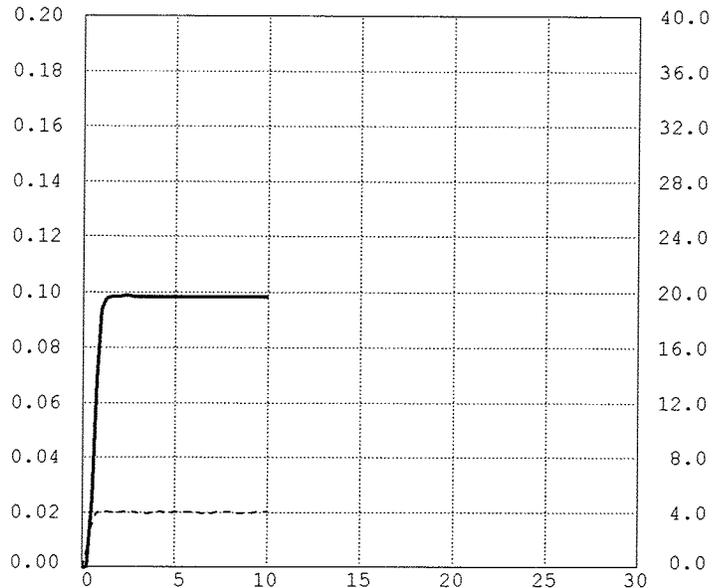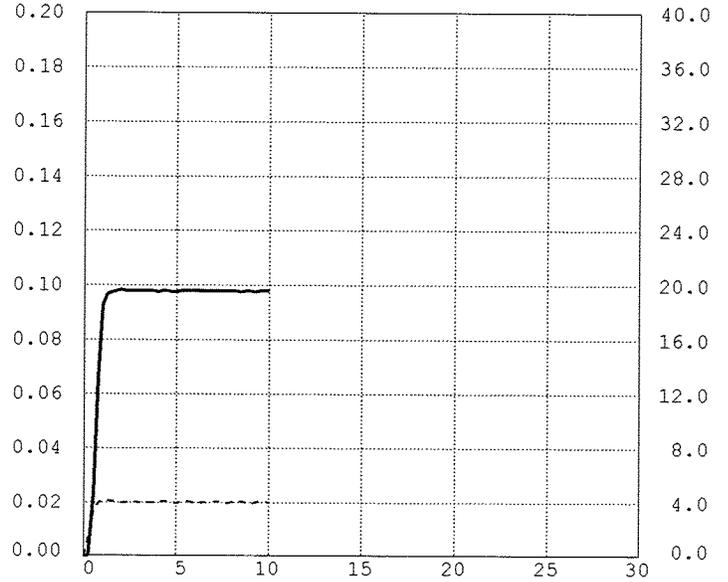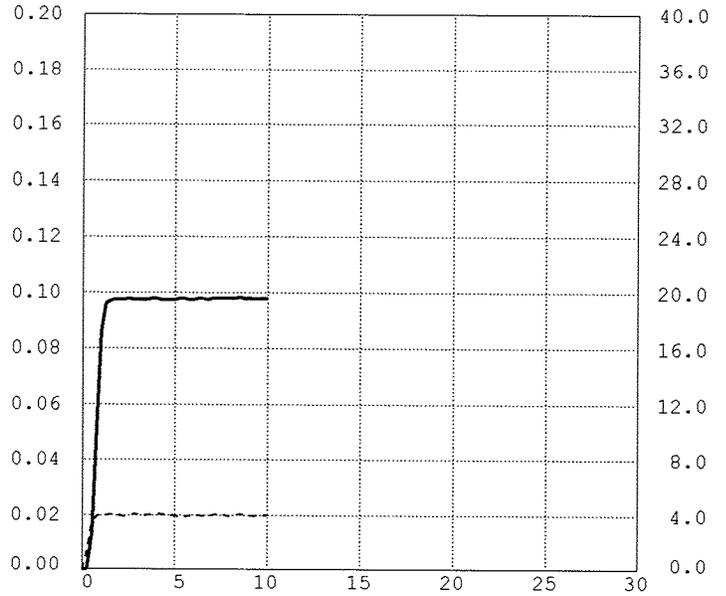

SW By J Bartlett

WC10 #162

09-24-13