

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 10/08/2013

Operator Name: RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13200

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:09
INTERNAL STANDARD	VERIFIED	22:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:09
BLANK TEST	0.00	22:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:10
BLANK TEST	0.00	22:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:11
BLANK TEST	0.00	22:12

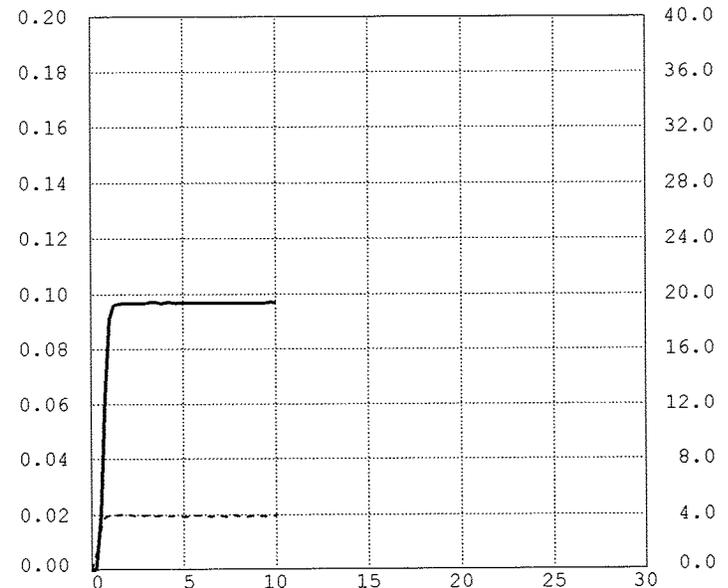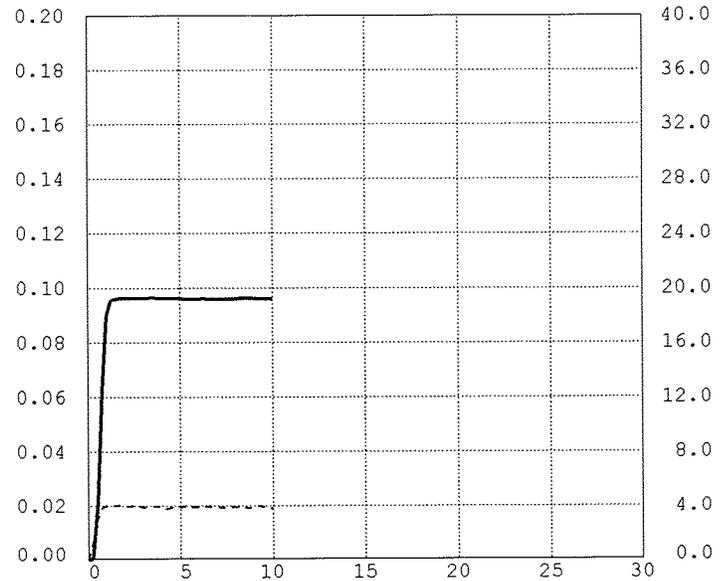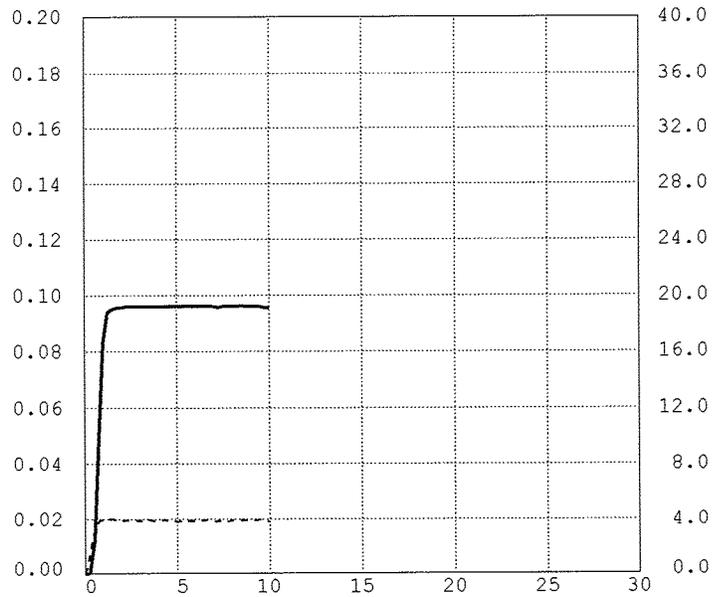

565 Rpt of Results were #162 10/08/13