

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 11/12/2013

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13200

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:25
INTERNAL STANDARD	VERIFIED	09:26
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:26
BLANK TEST	0.00	09:27
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	09:27
BLANK TEST	0.00	09:28
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	09:28
BLANK TEST	0.00	09:29

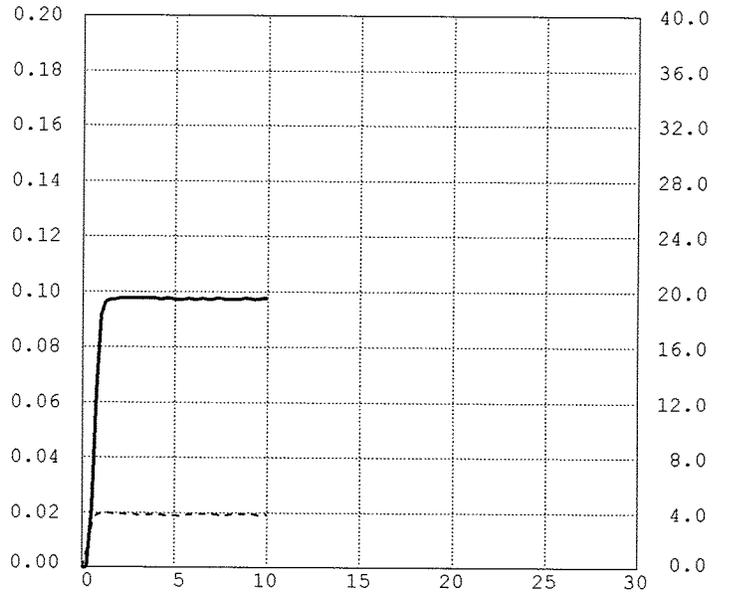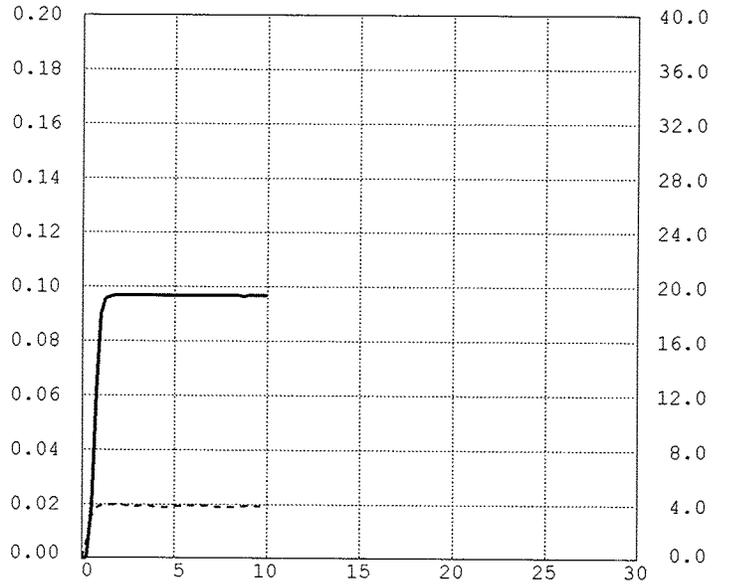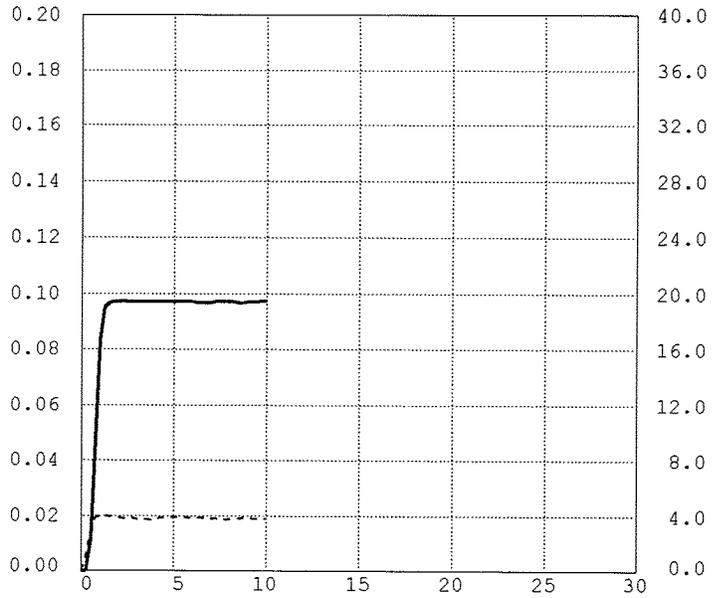

J. Charles B. Geisler #245 11/12/13 0929