

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 12/01/2013

Operator Name: CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 13260

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:01
INTERNAL STANDARD	VERIFIED	11:01
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:01
BLANK TEST	0.00	11:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:03
BLANK TEST	0.00	11:03
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	11:04
BLANK TEST	0.00	11:04

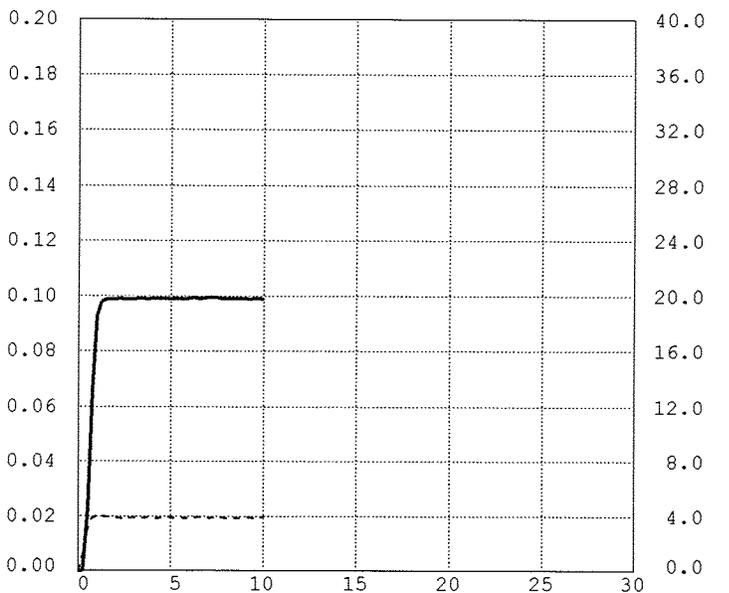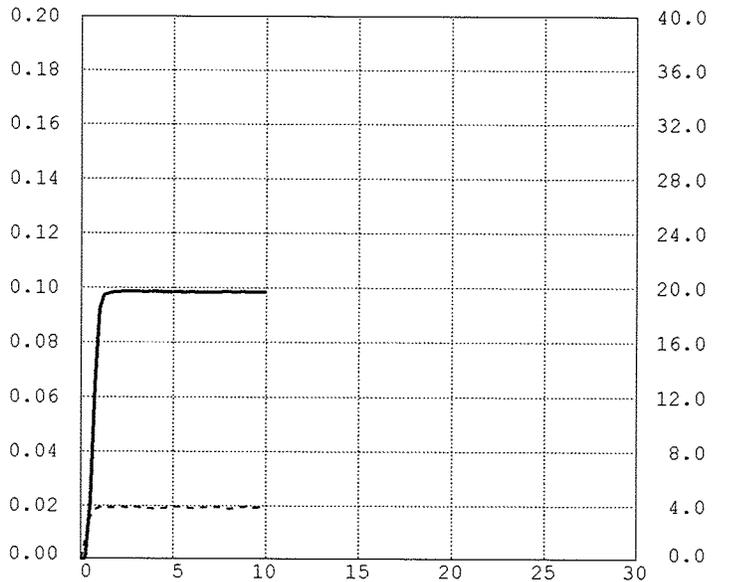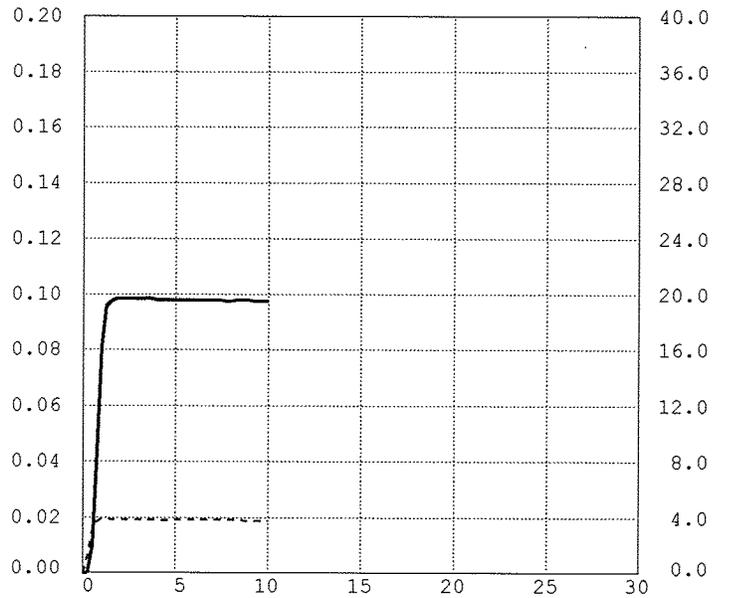

Charles B. Geisler
#248 12/01/13
1106