

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/06/2014

Operator Name: RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 13260

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 00:56 |
| INTERNAL STANDARD       | VERIFIED | 00:56 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 00:56 |
| BLANK TEST              | 0.00     | 00:57 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 00:57 |
| BLANK TEST              | 0.00     | 00:58 |
| REFERENCE STANDARD TEMP | 33.96c   |       |
| REFERENCE STANDARD      | 0.09     | 00:58 |
| BLANK TEST              | 0.00     | 00:59 |

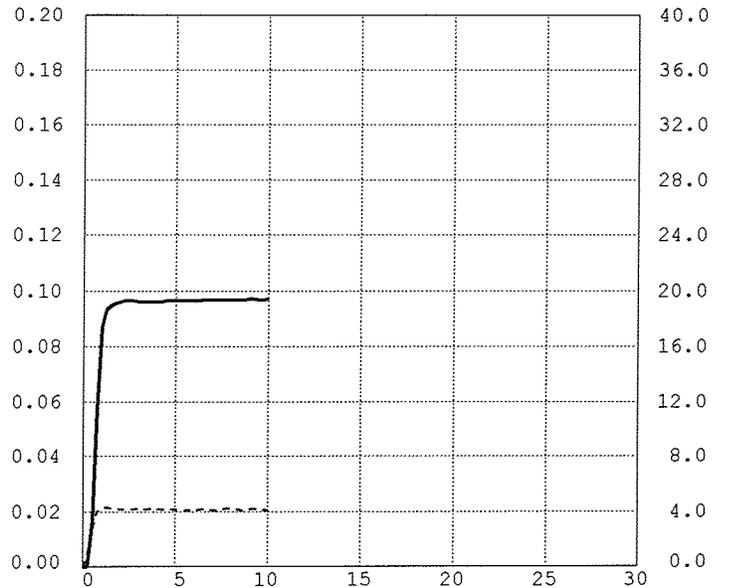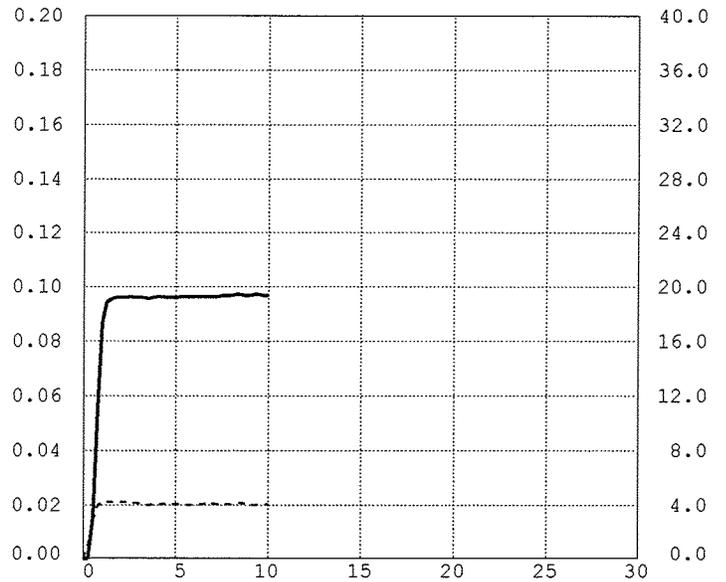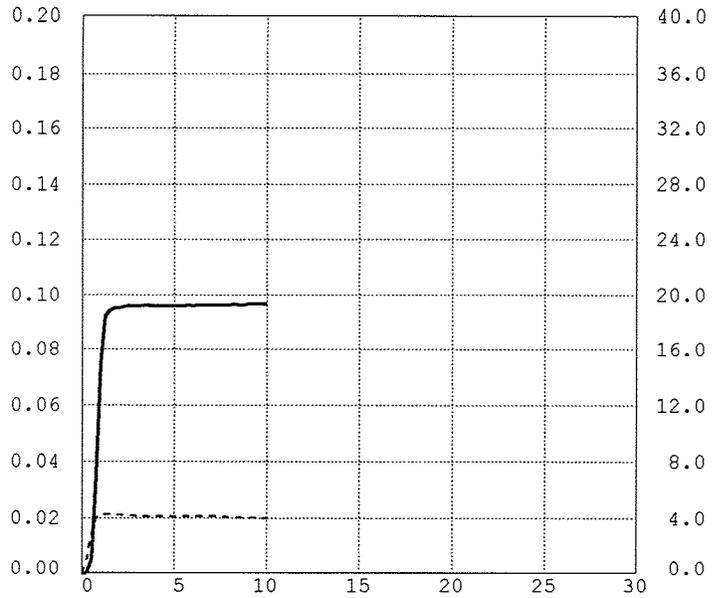

505 Rpt of Bartlett WESO #162 01-06-14