

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/15/2014

Operator Name: RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14080

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:01
INTERNAL STANDARD	VERIFIED	01:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:02
BLANK TEST	0.00	01:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:03
BLANK TEST	0.00	01:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:04
BLANK TEST	0.00	01:04

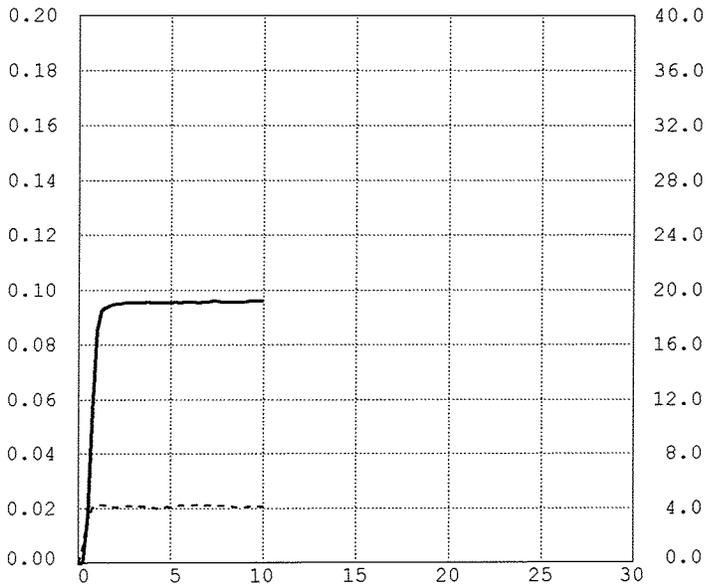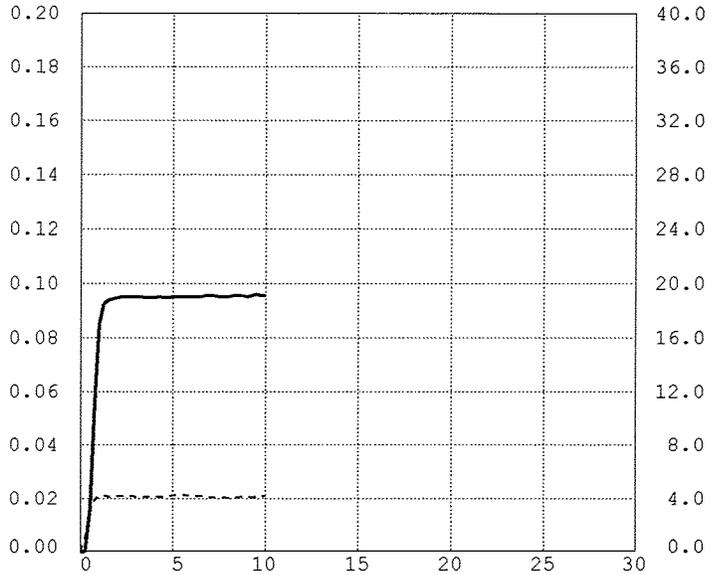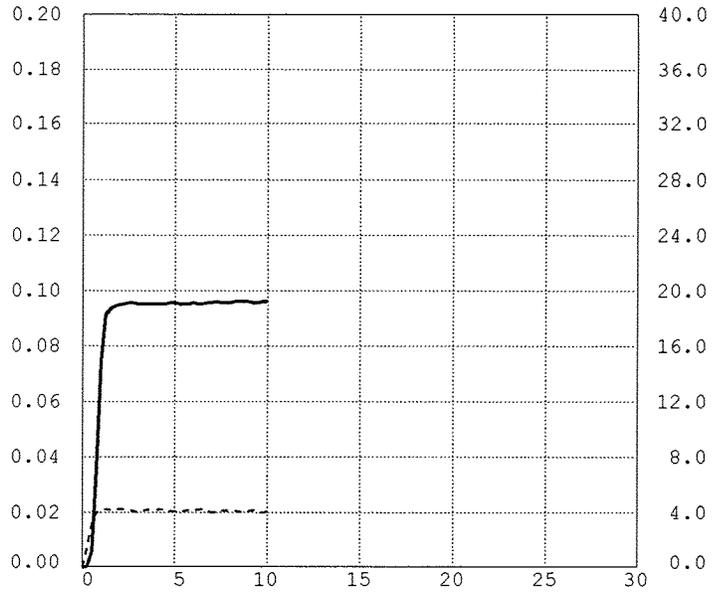

See *Ralph Bartlett* memo #162 07-15-14