

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 07/21/2014

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14080

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:17
INTERNAL STANDARD	VERIFIED	10:17
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	10:18
BLANK TEST	0.00	10:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:19
BLANK TEST	0.00	10:19
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	10:20
BLANK TEST	0.00	10:20

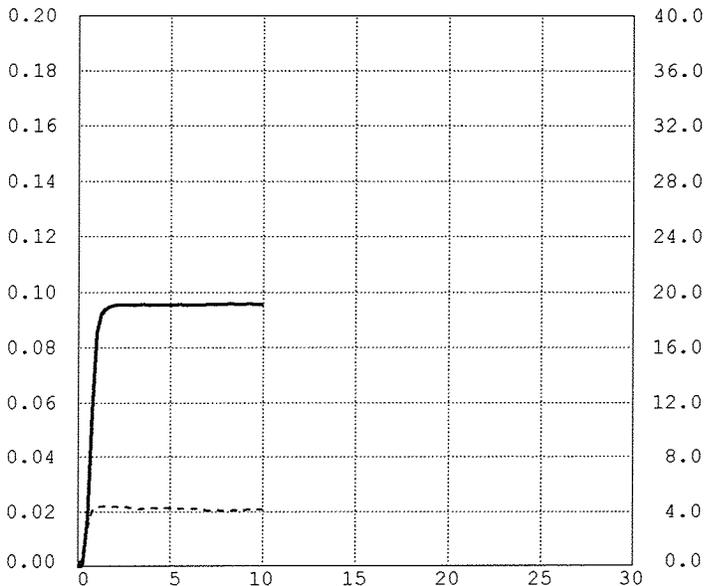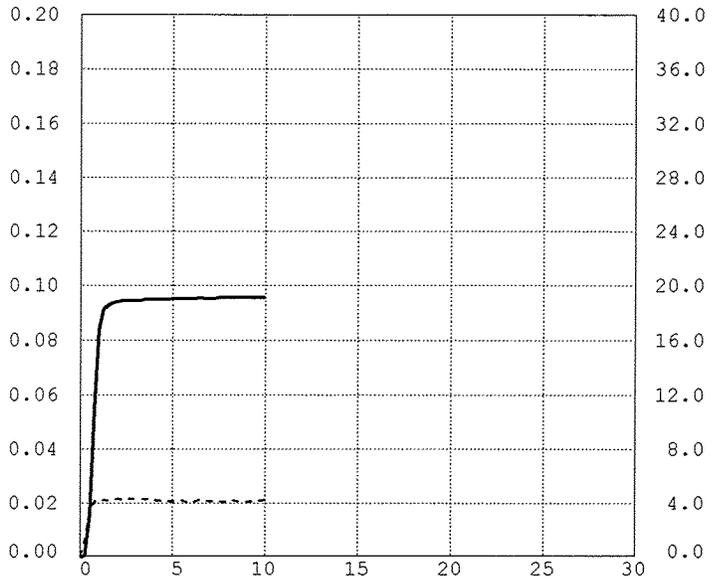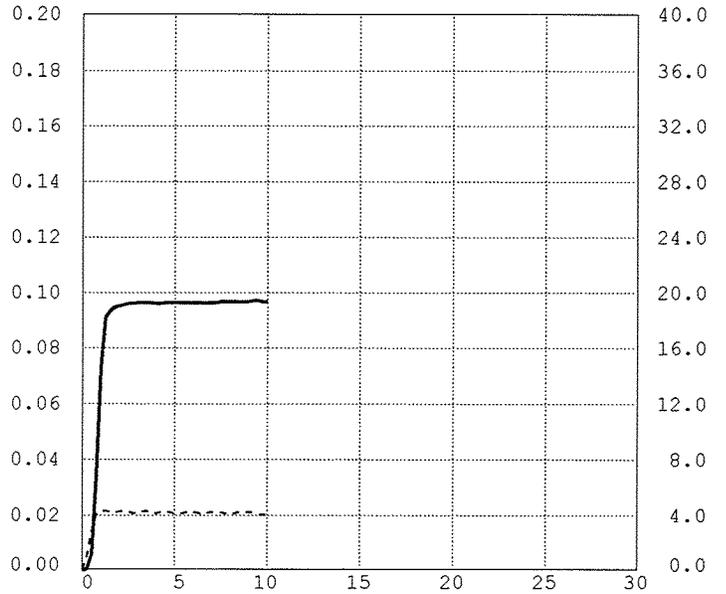

*C. B. Geisler*  
#248  
7/21/14 1021