

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 09/01/2014

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:03
INTERNAL STANDARD	VERIFIED	01:04
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	01:04
BLANK TEST	0.00	01:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:06
BLANK TEST	0.00	01:07
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:07
BLANK TEST	0.00	01:08

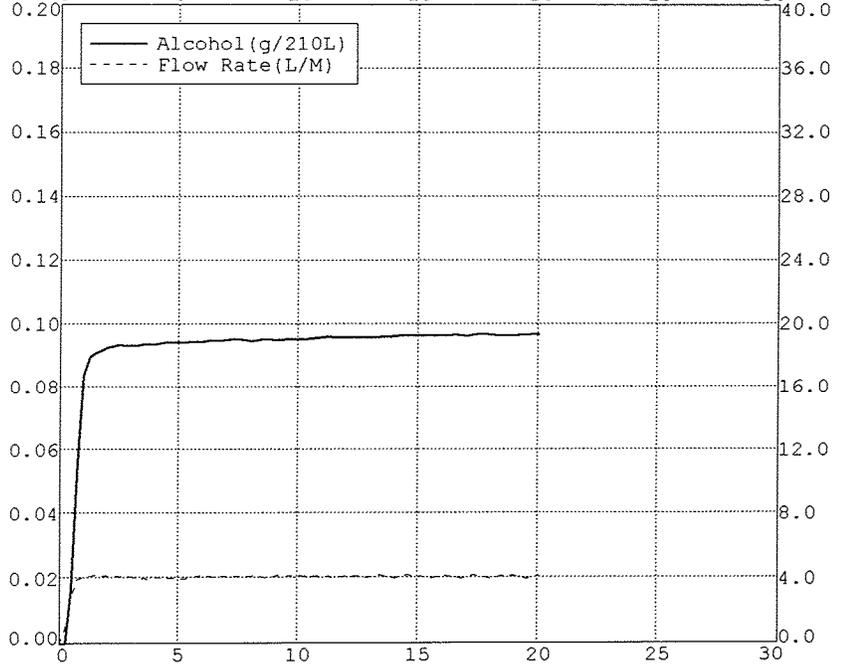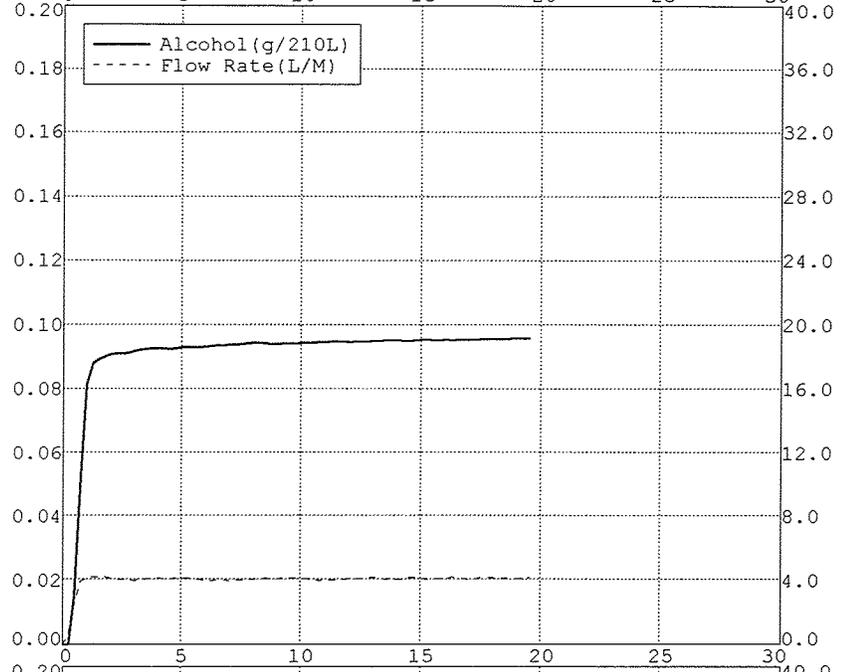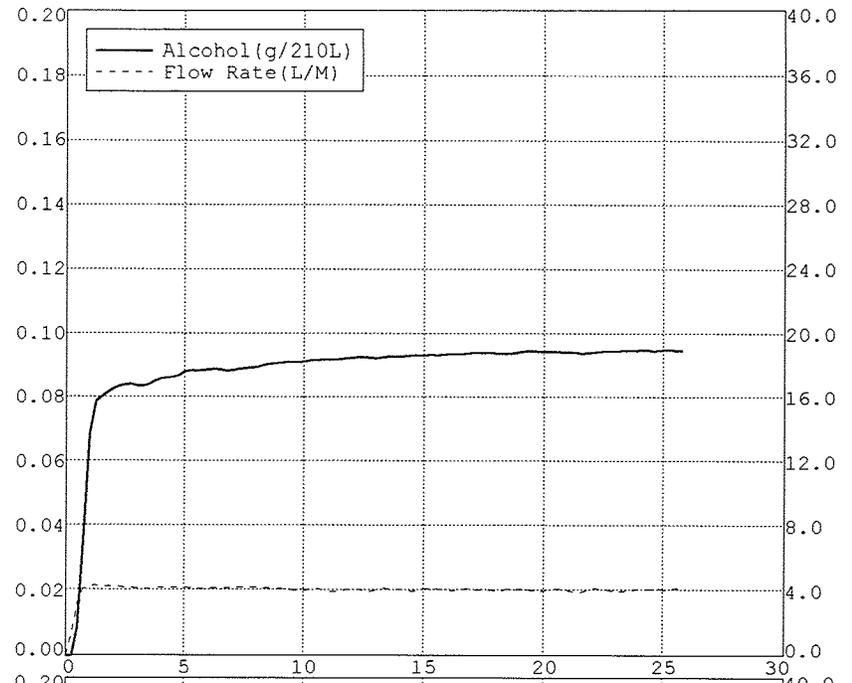

*SGS RJ Bartlett WSO #162*  
*09-01-14*