

SUPERVISOR TEST



WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 09/09/2014

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14140

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:13
INTERNAL STANDARD	VERIFIED	02:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:14
BLANK TEST	0.00	02:15
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:15
BLANK TEST	0.00	02:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:16
BLANK TEST	0.00	02:17

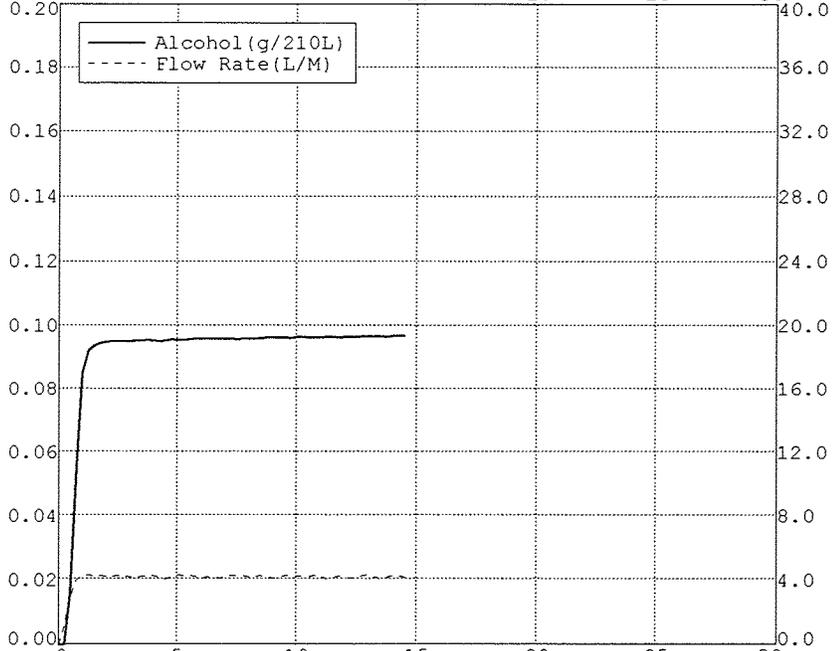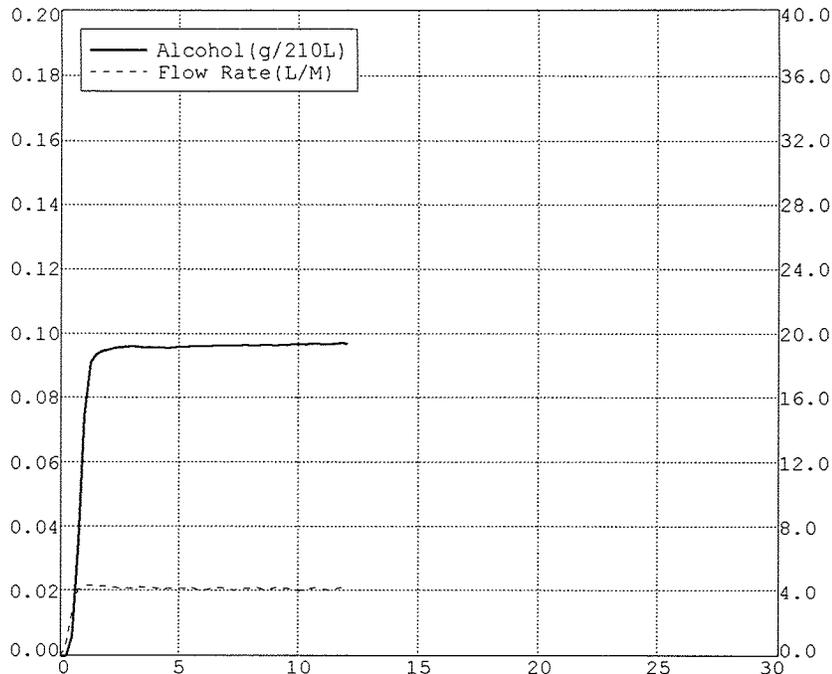

SGR BY *R. Bartlett* WCSO #162  
09-09-14