

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/15/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:51
INTERNAL STANDARD	VERIFIED	01:51
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	01:51
BLANK TEST	0.00	01:52
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:52
BLANK TEST	0.00	01:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:54
BLANK TEST	0.00	01:55

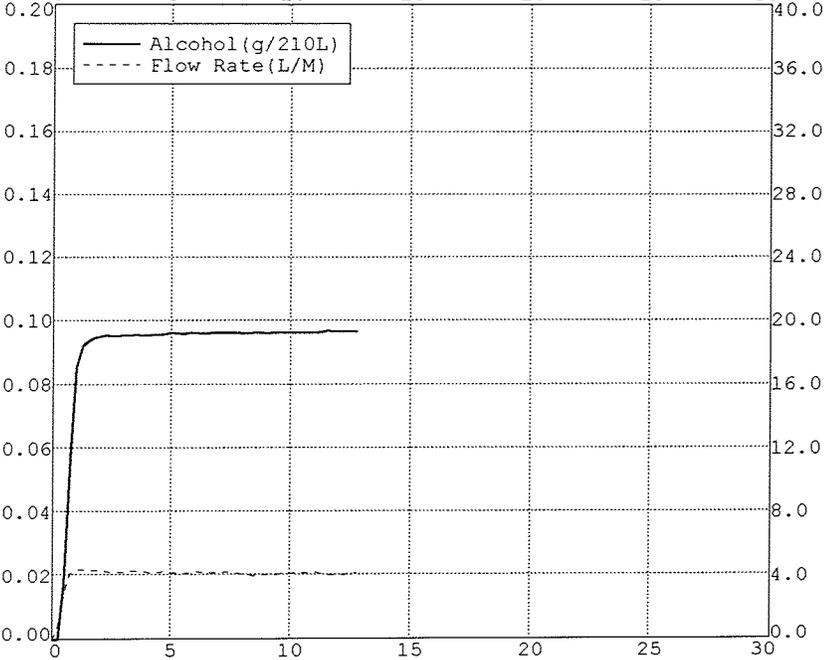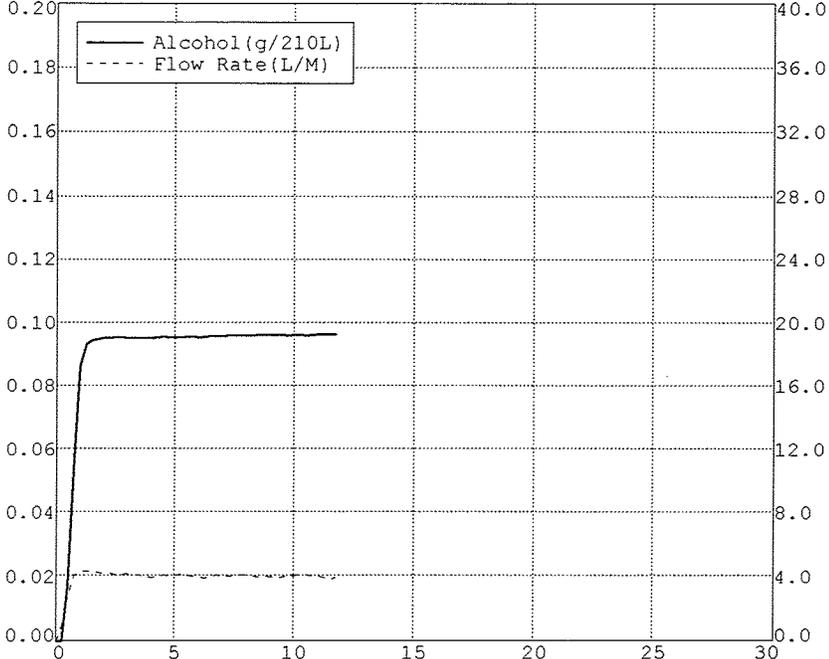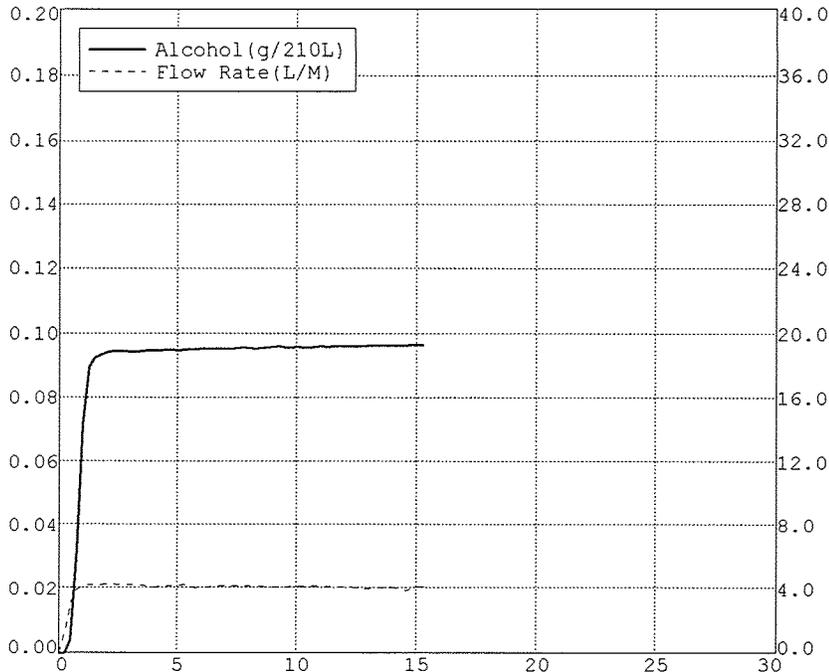

SGS Rly Bartlett

WCSO #162 09-15-14