

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/16/2014

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14180

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:04
INTERNAL STANDARD	VERIFIED	09:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:04
BLANK TEST	0.00	09:05
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	09:05
BLANK TEST	0.00	09:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:07
BLANK TEST	0.00	09:08

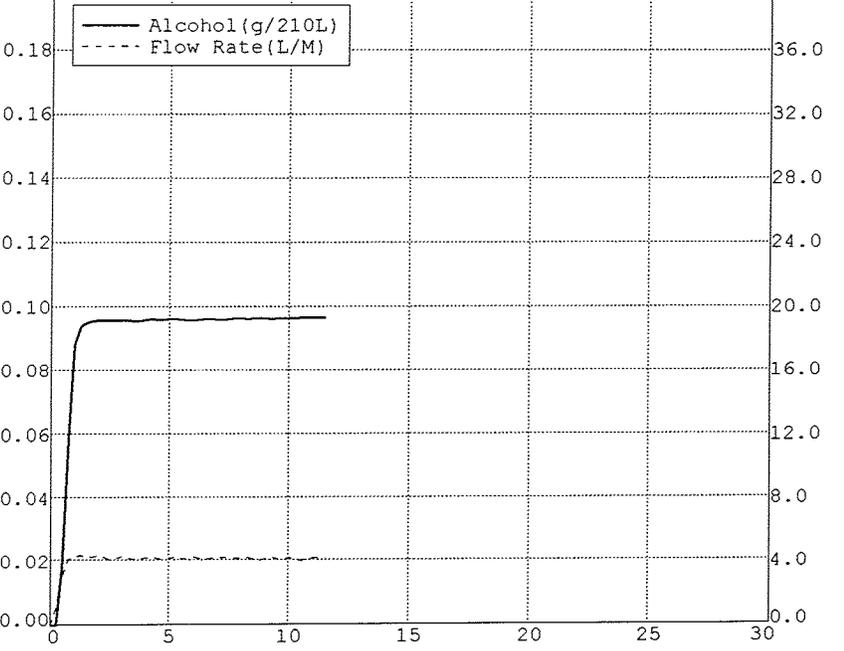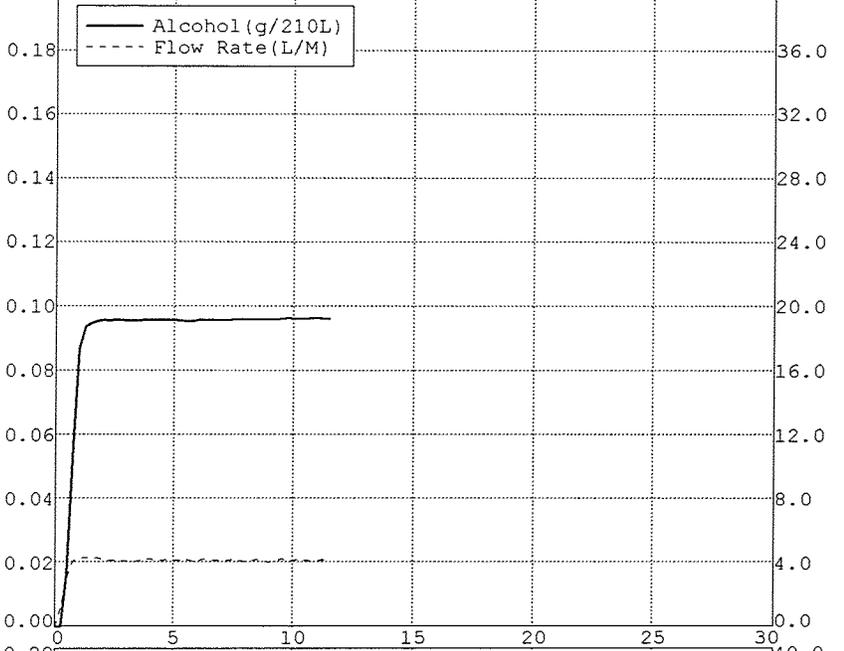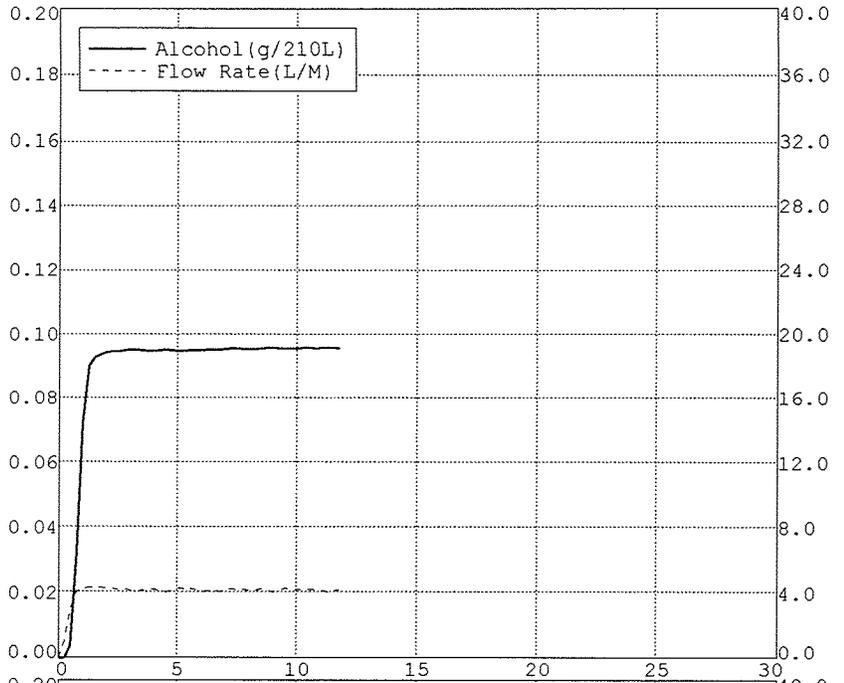

Charles B. Geisler #215