

SUPERVISOR TEST



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/24/2014

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:26
INTERNAL STANDARD	VERIFIED	12:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:27
BLANK TEST	0.00	12:28
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:28
BLANK TEST	0.00	12:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:29
BLANK TEST	0.00	12:30

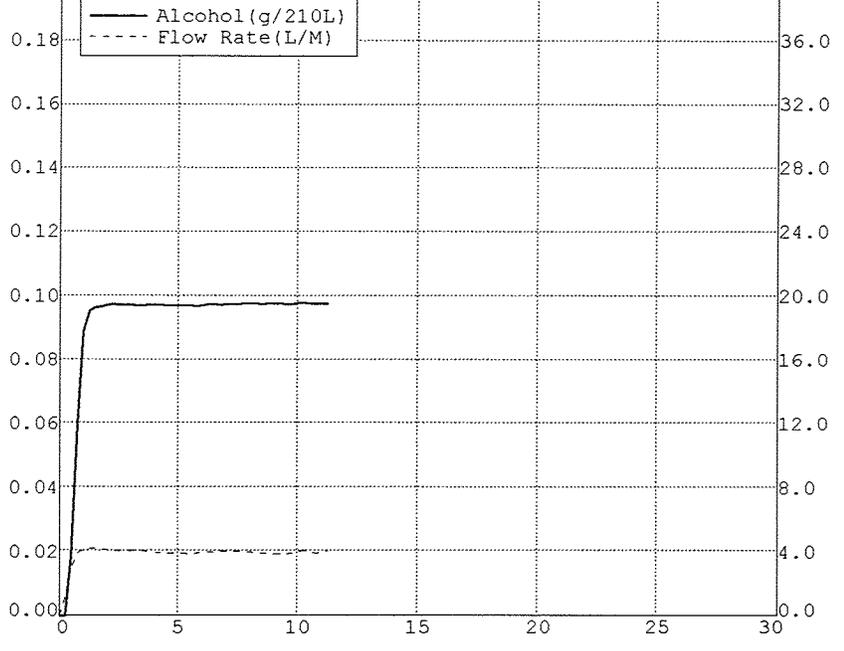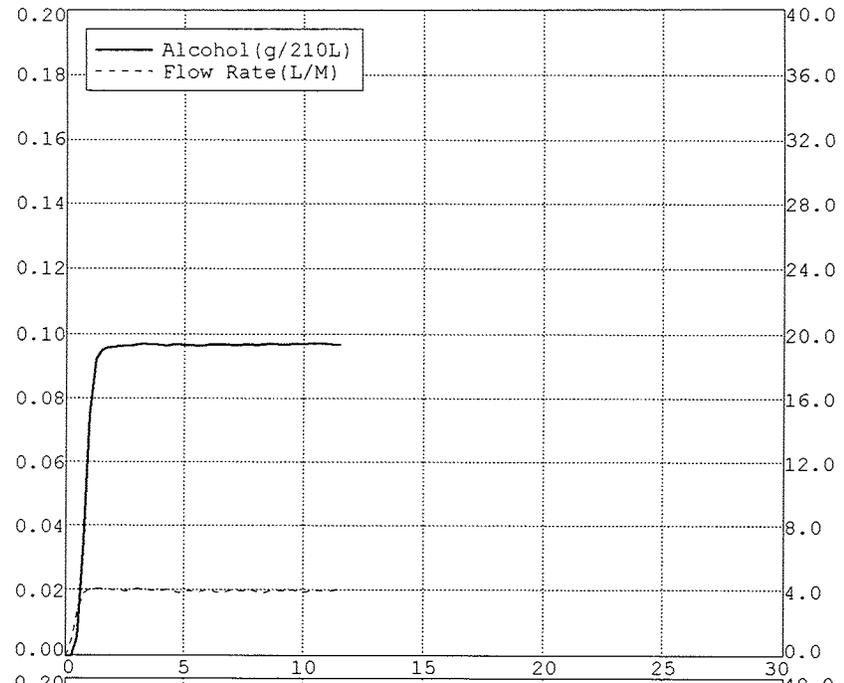

Charles B. Geisler #2014