

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/02/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:22
INTERNAL STANDARD	VERIFIED	01:22
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	01:22
BLANK TEST	0.00	01:23
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:24
BLANK TEST	0.00	01:24
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	01:25
BLANK TEST	0.00	01:26

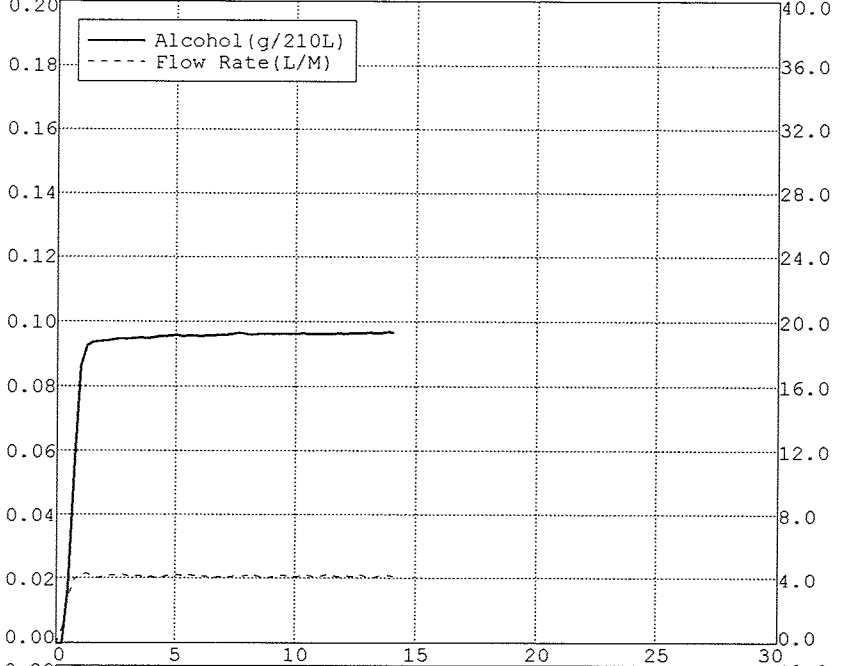

SGS R.J. Bartlett WPSO #162

12-07-14