

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/08/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:07
INTERNAL STANDARD	VERIFIED	00:07
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:08
BLANK TEST	0.00	00:09
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:09
BLANK TEST	0.00	00:10
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	00:10
BLANK TEST	0.00	00:11

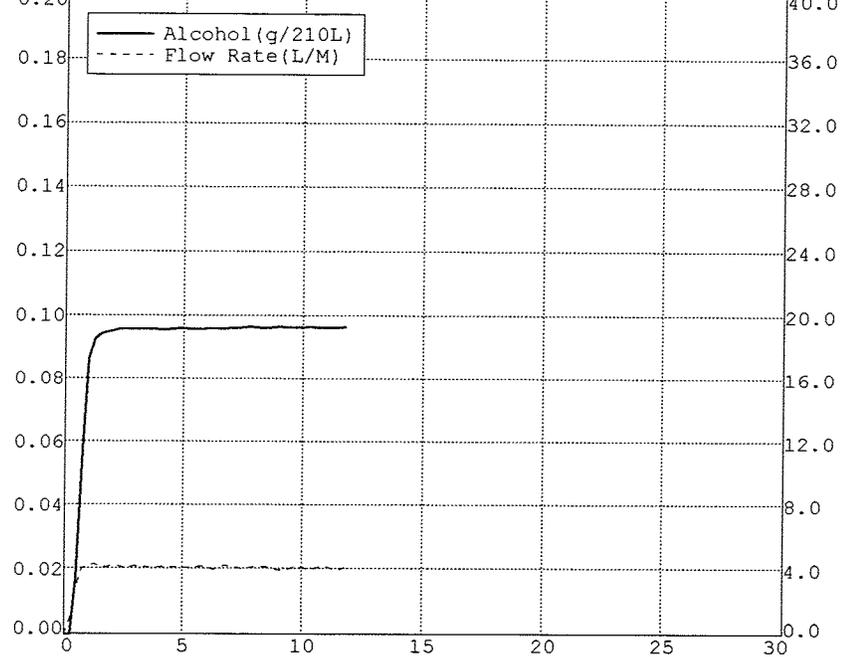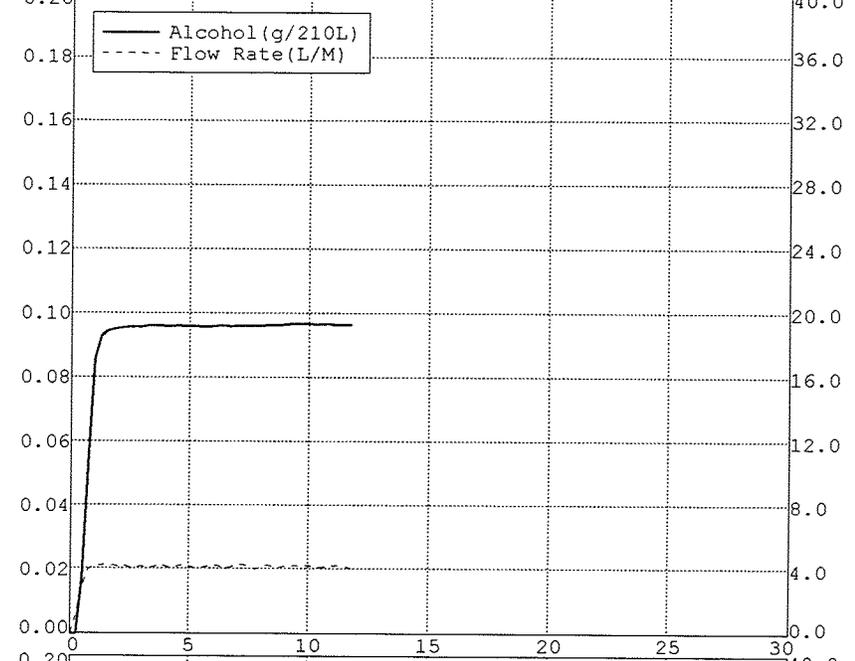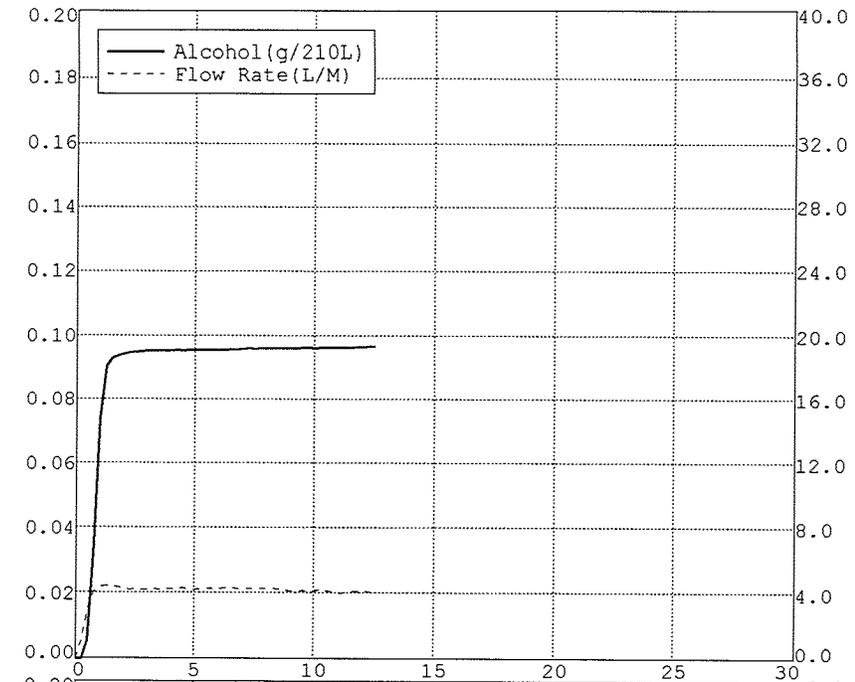

*SGS Bartlett J Bartlett WESO #162
12/08/14*