

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 12/22/2014

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:17
INTERNAL STANDARD	VERIFIED	00:17
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:17
BLANK TEST	0.00	00:18
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:18
BLANK TEST	0.00	00:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:20
BLANK TEST	0.00	00:21

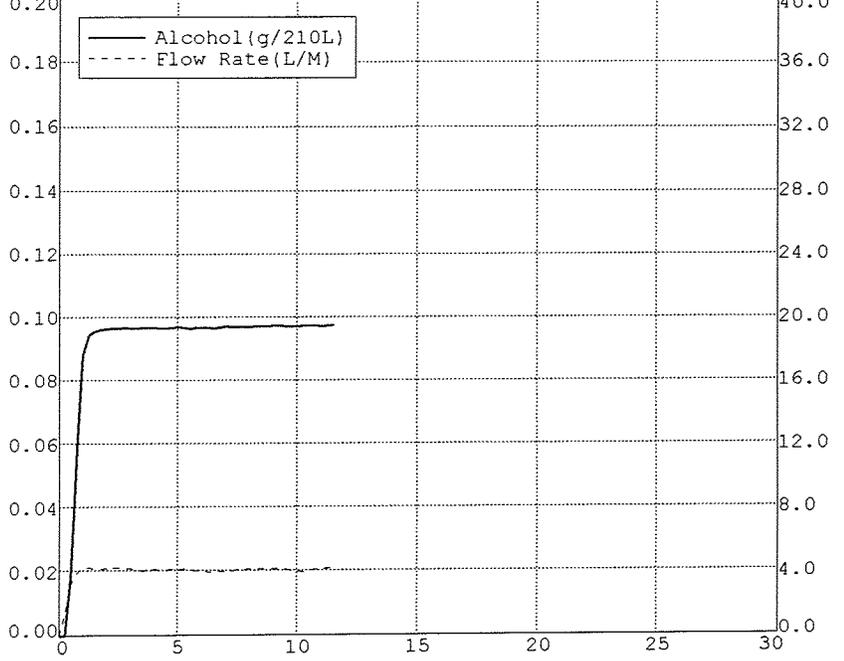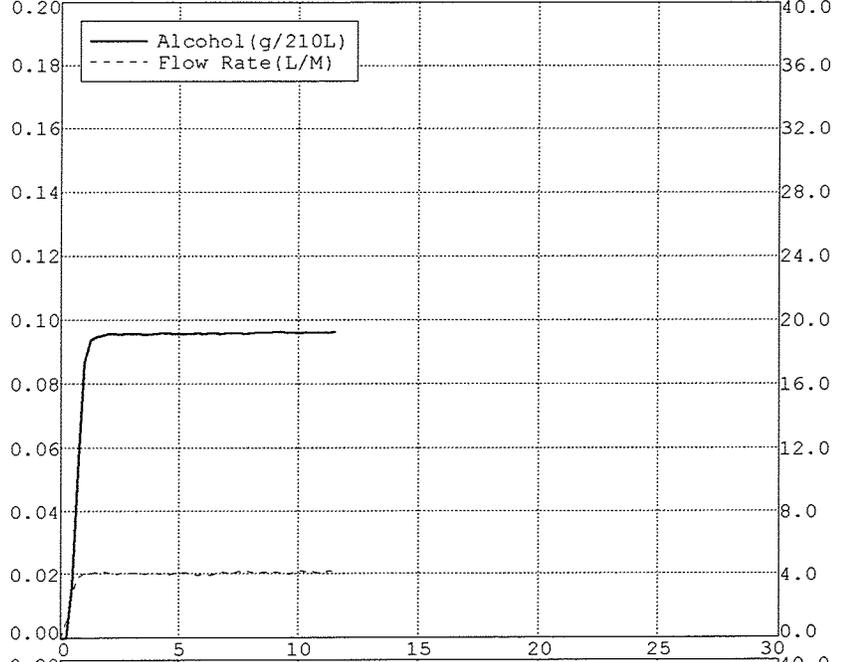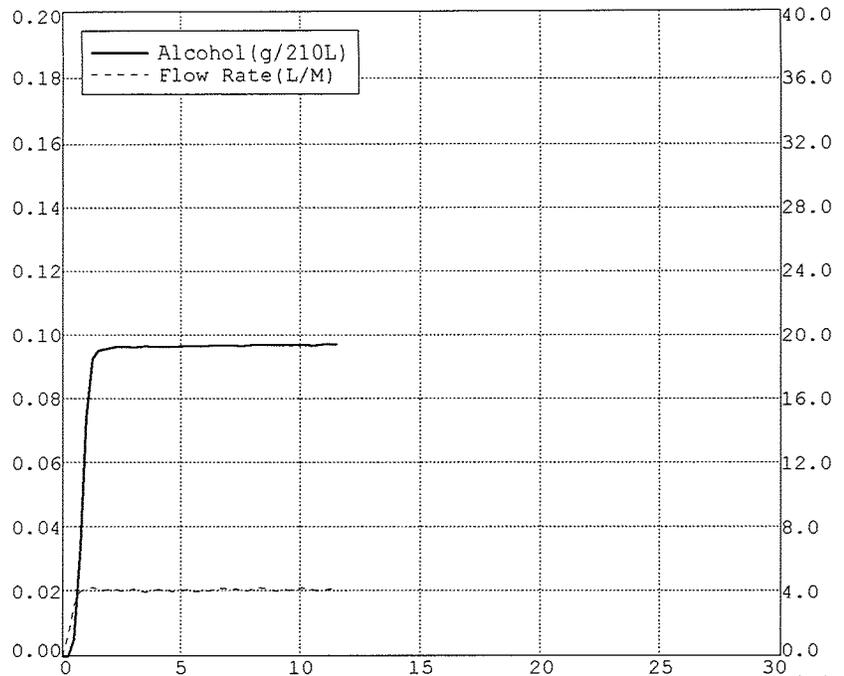

*See Ralph J Bartlett Wes #16c
 12-22-14*