

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 03/27/2014

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 13320

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:25
INTERNAL STANDARD	VERIFIED	11:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:25
BLANK TEST	0.00	11:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:26
BLANK TEST	0.00	11:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:28
BLANK TEST	0.00	11:29

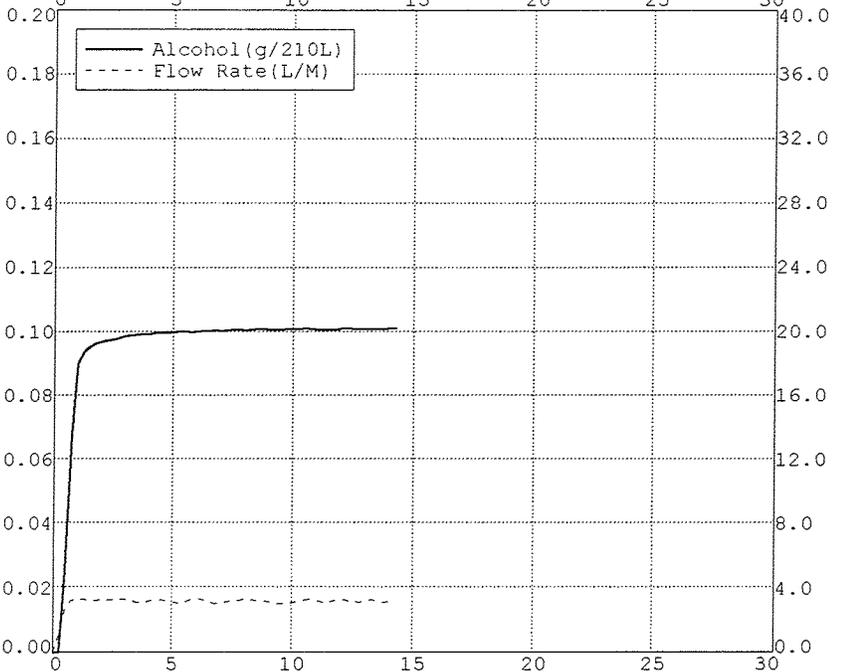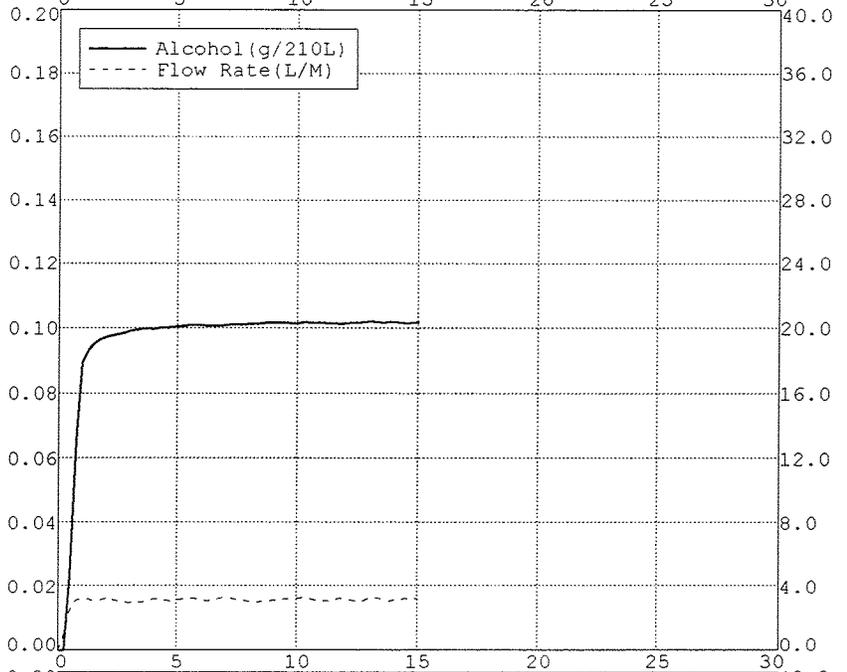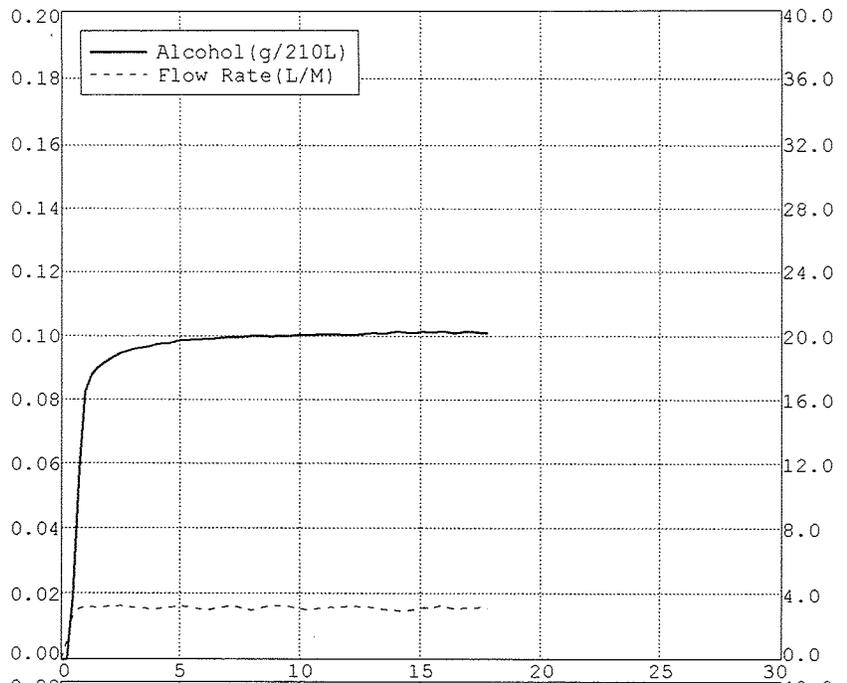

*Handwritten signature and notes:*  
C. B. Geisler #248 3/27/14 11:29 AM