

# SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 04/07/2014

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14040

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 13:35 |
| INTERNAL STANDARD       | VERIFIED | 13:35 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 13:35 |
| BLANK TEST              | 0.00     | 13:36 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 13:36 |
| BLANK TEST              | 0.00     | 13:37 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 13:38 |
| BLANK TEST              | 0.00     | 13:38 |

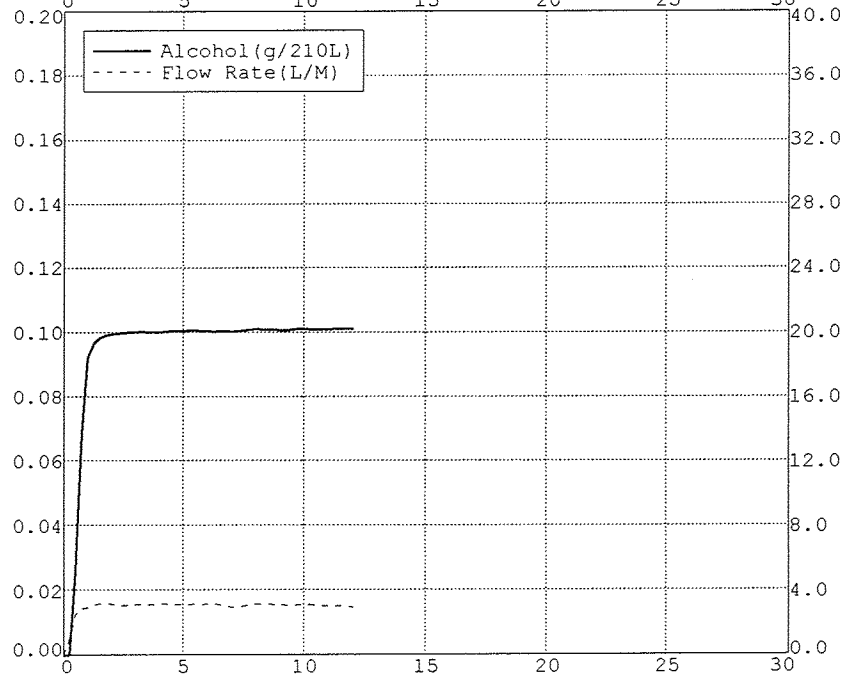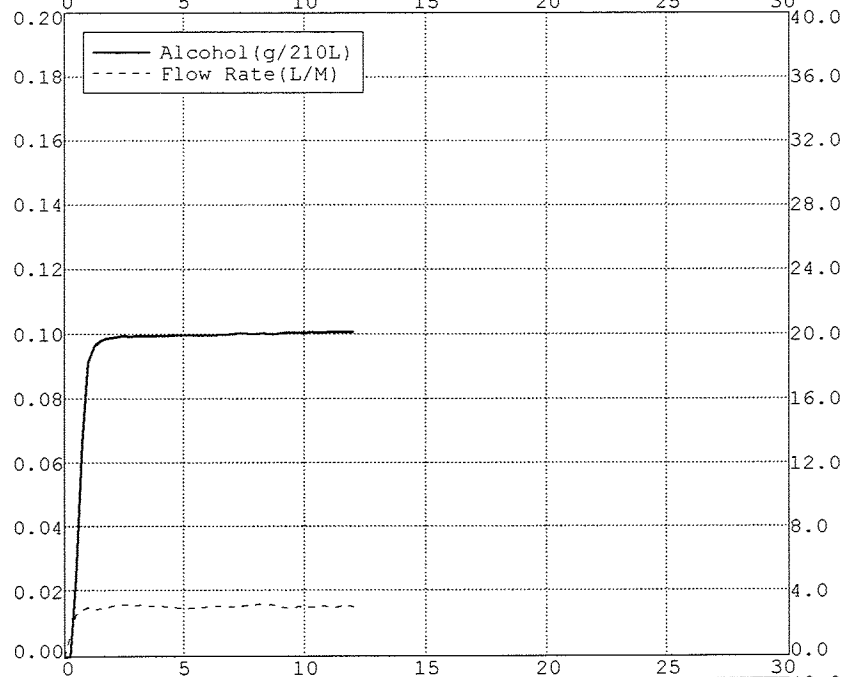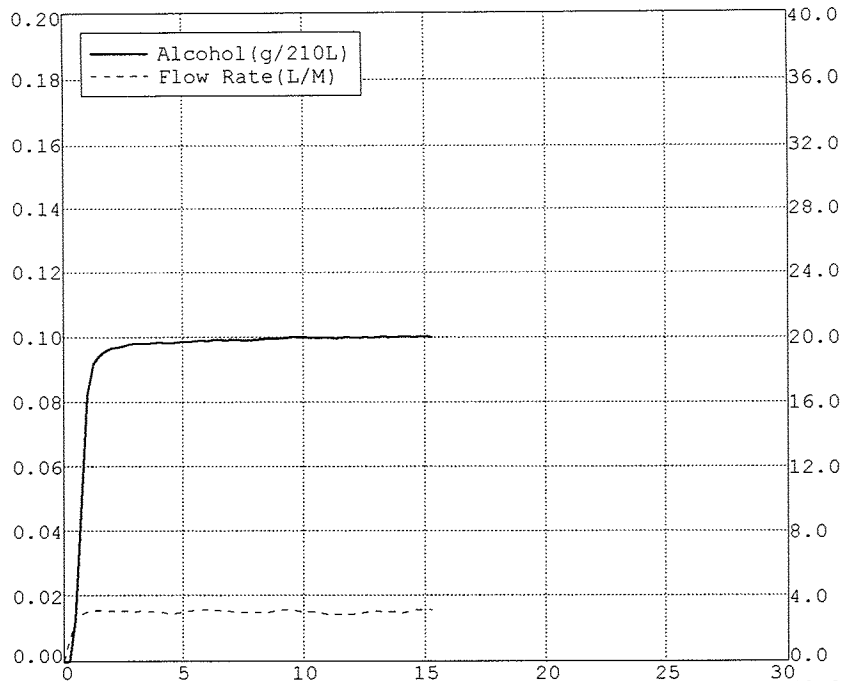

SGS B&J Bartlett WESU #162

04-07-14