

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 04/14/2014

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 14040

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:18
INTERNAL STANDARD	VERIFIED	03:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:18
BLANK TEST	0.00	03:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:19
BLANK TEST	0.00	03:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:21
BLANK TEST	0.00	03:22

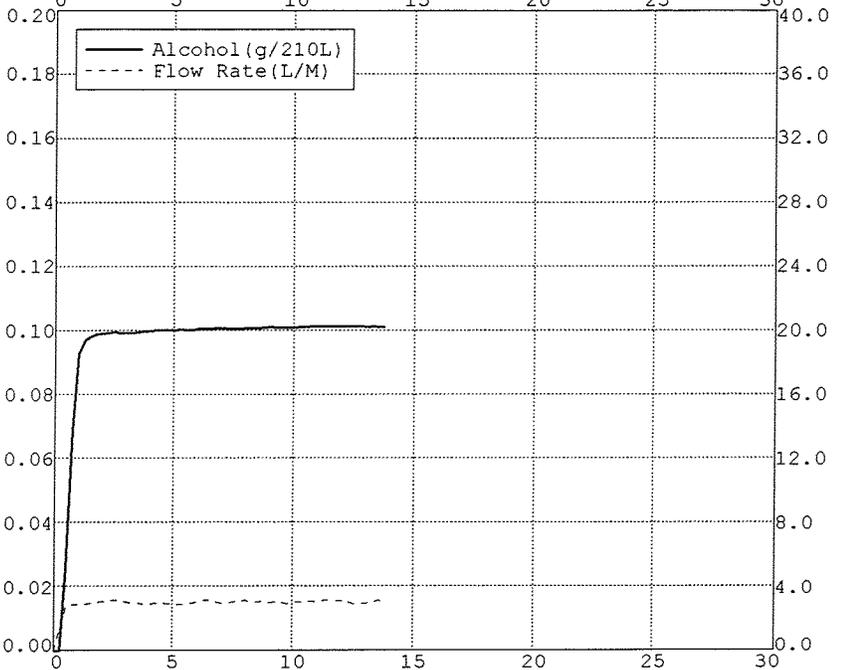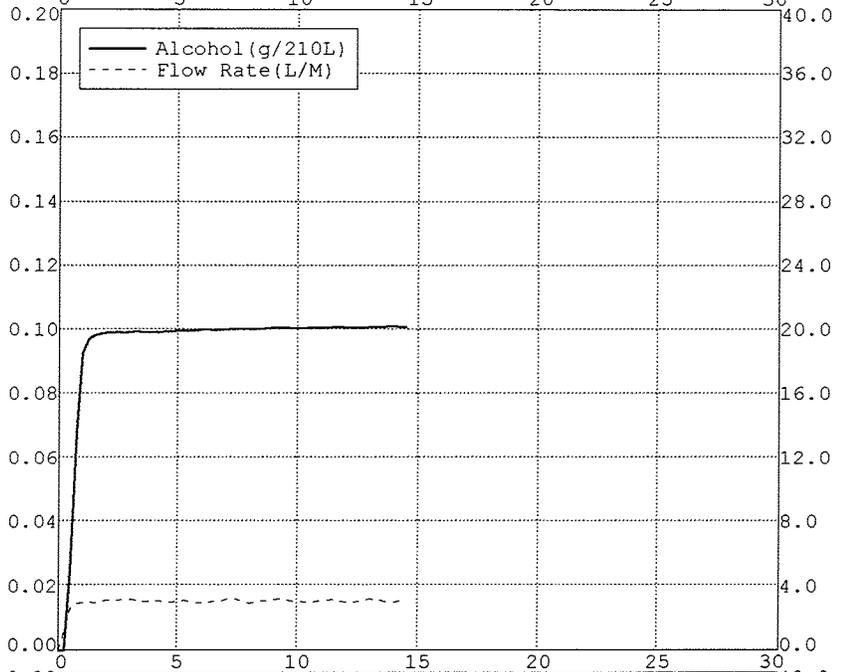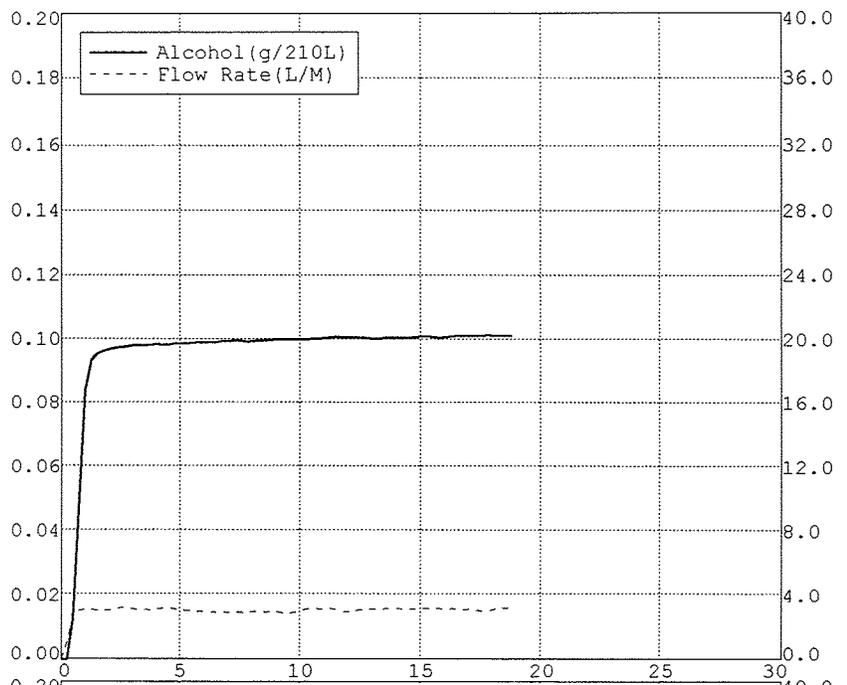

S/S RJA Bartlett were #166 - 04-14-14