

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/23/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14040

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:26
INTERNAL STANDARD	VERIFIED	03:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:27
BLANK TEST	0.00	03:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	03:28
BLANK TEST	0.00	03:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:29
BLANK TEST	0.00	03:30

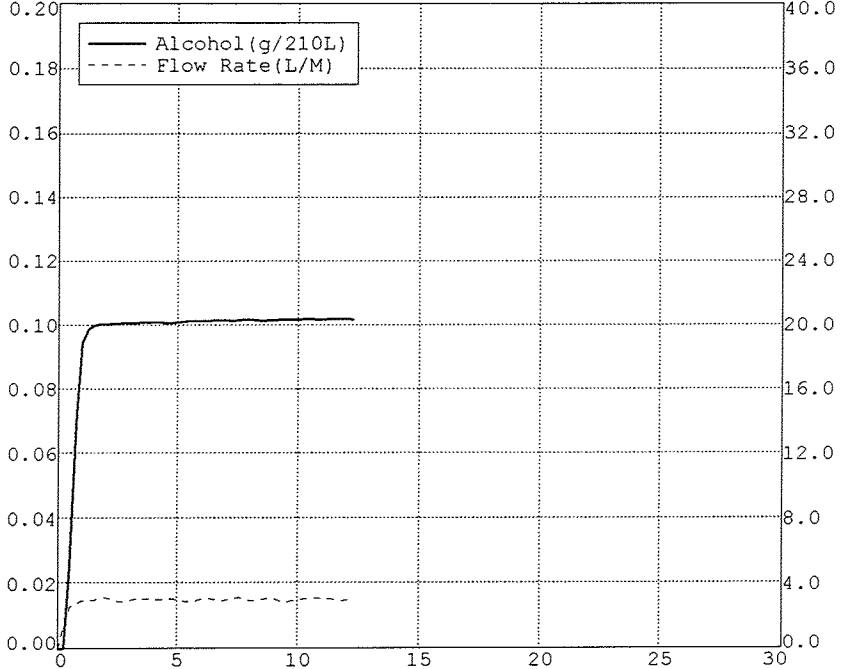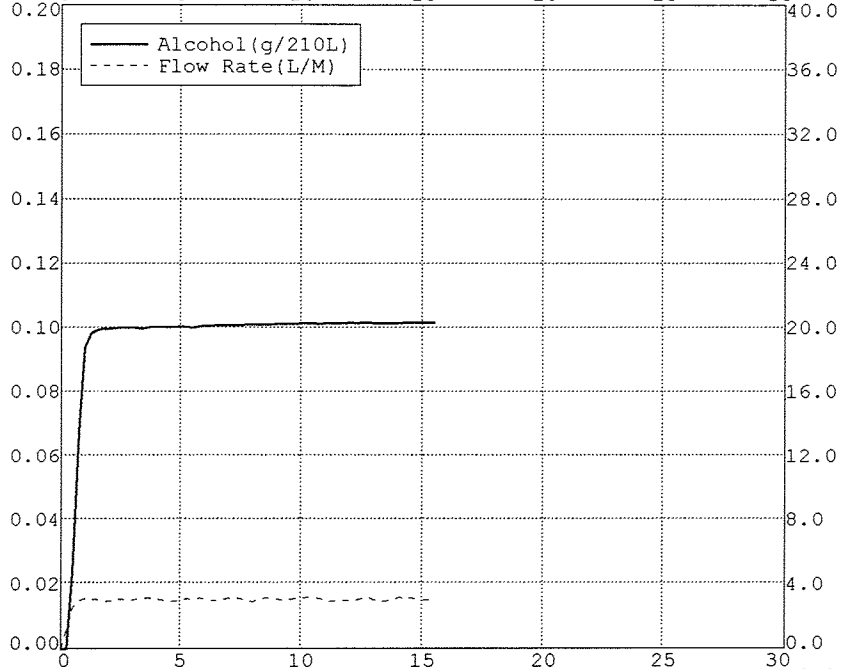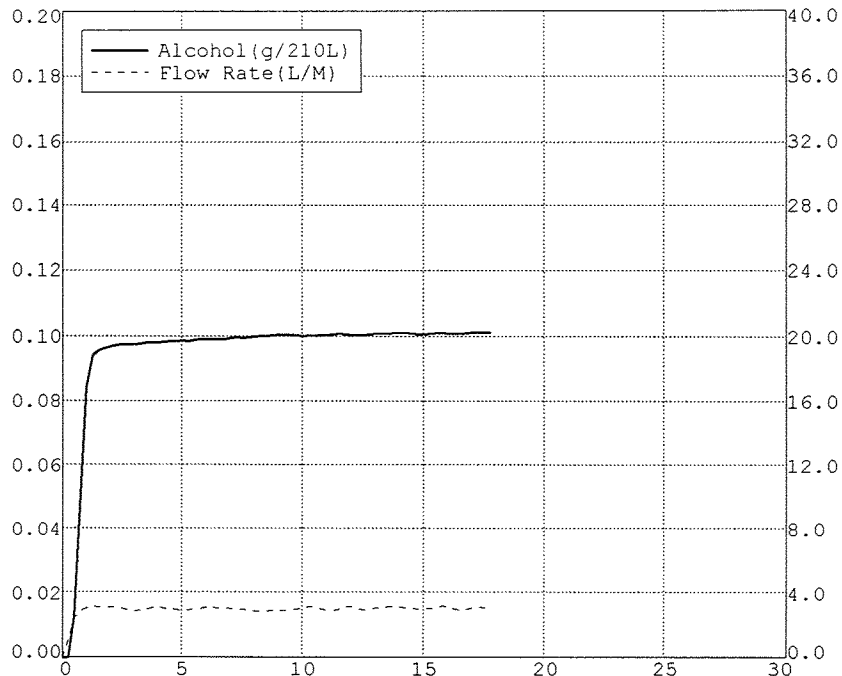

Set by Bartlett WCO #162 04-23-14