

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 05/07/2014

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14040

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:05
INTERNAL STANDARD	VERIFIED	03:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:06
BLANK TEST	0.00	03:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:07
BLANK TEST	0.00	03:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:08
BLANK TEST	0.00	03:09

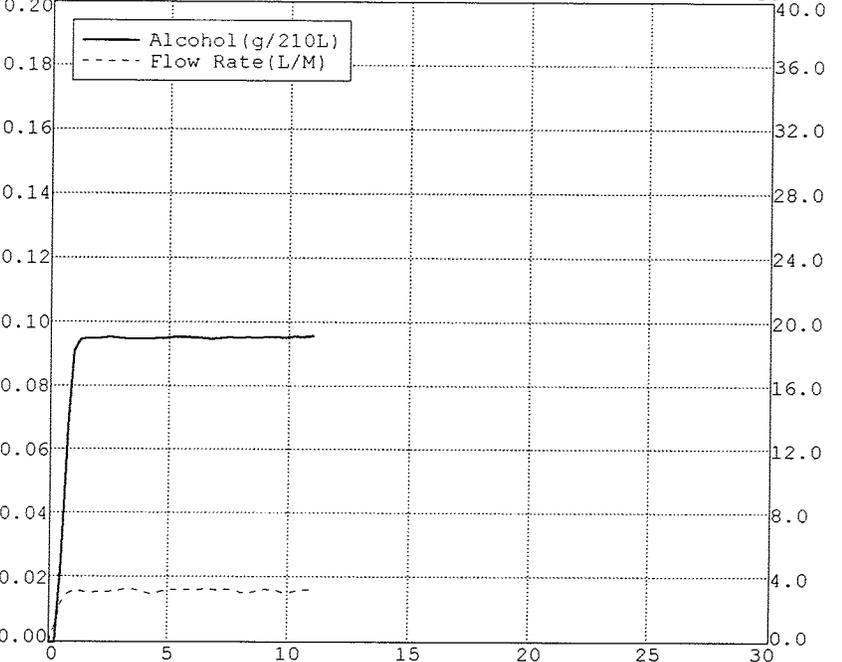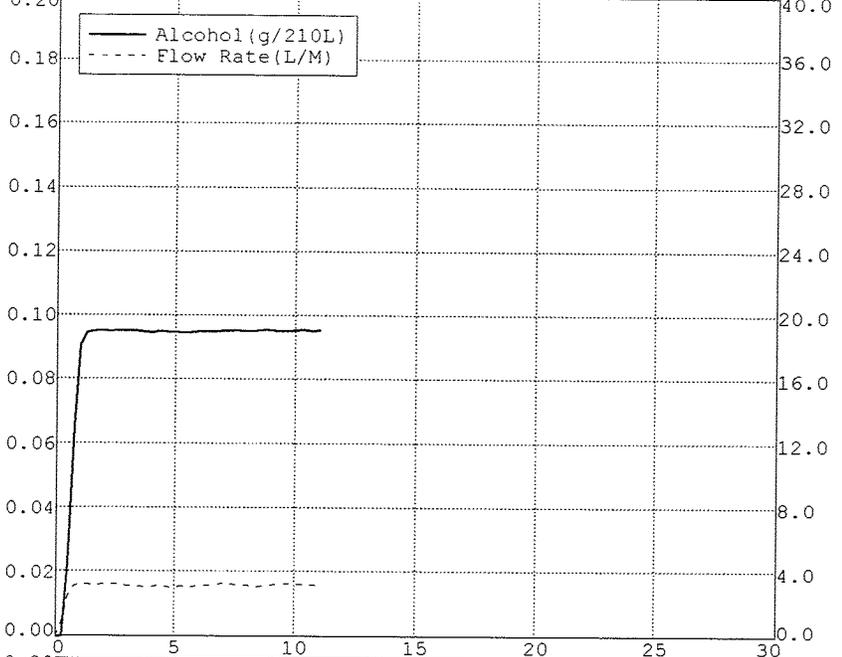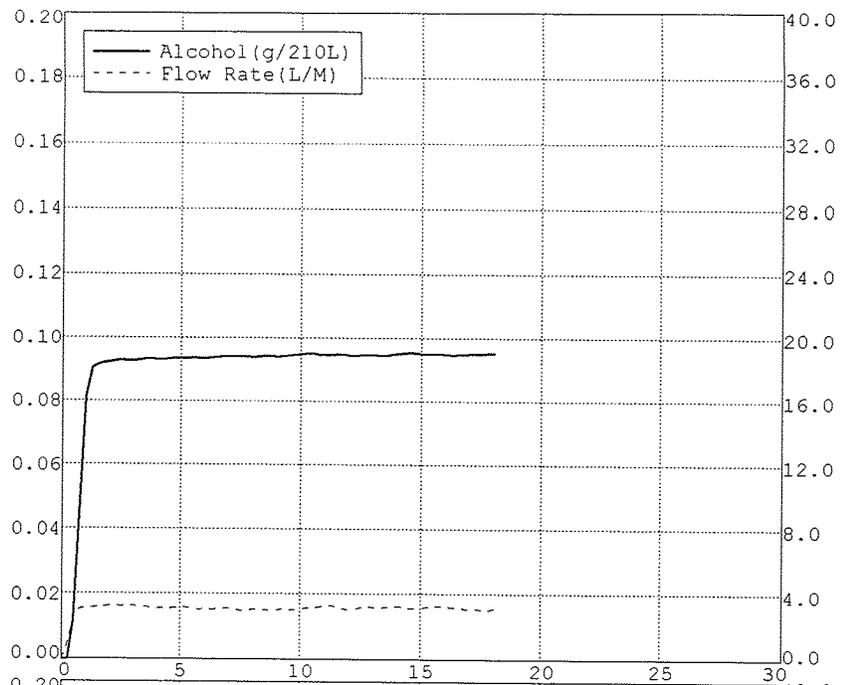

SGT R.J. Bartlett WOSO # 162

05-07-14